

# State Practices in the Use of Bituminous Concrete

W. E. CHASTAIN, SR., Engineer of Physical Research, and  
JOHN E. BURKE, Assistant Engineer of Physical Research  
Bureau of Research and Planning, Illinois Division of Highways

● FIFTY highway agencies cooperated in furnishing the information on bituminous concrete practice that is presented and summarized in this report. Cooperating agencies include all of the state highway departments, the District of Columbia Department of Highways, and the Ontario (Canada) Department of Highways. The contributions of all of these agencies are gratefully acknowledged.

The information that is herein compiled was assembled to serve as a basis upon which to pattern the construction of the experimental flexible pavement to be tested during the AASHO Road Test. Two separate questionnaires were sent out to and completed by the cooperating agencies in 1953. The first questionnaire was of a general nature and the second was much more detailed. Data from the two questionnaires were tabulated and the tabulations were submitted to all of the cooperating agencies for checking and for adding information to bring the tabulations up-to-date for 1954. The practice represented in this report is therefore 1954 practice.

Although the questionnaires were considered to be "bituminous concrete" questionnaires, which would include both tar and asphaltic concrete, they were definitely pointed toward asphaltic-concrete usage since there was no question but that asphaltic concrete rather than tar concrete would more truly represent national practice and be used in the Test Road construction. However, much of the information that has been compiled applies to both types of bituminous concrete.

In preparing the questionnaires it was assumed that bituminous concrete as generally used consists of a mixture of coarse aggregate, fine aggregate, mineral filler and asphalt cement. Such a material is plant-mixed, laid with a spreading and finishing machine, and immediately compacted with rollers. With one or two possible exceptions, all of the reporting agencies make some use of such a material. However, considerable variation occurs in the number of refinements that are introduced and the degree of control that is exercised. Practice is tailored generally to meet the individual needs of the constructing agencies. For example, a bituminous-concrete mixture that is to be subjected to the heavy traffic and severe moisture conditions of one area must meet much higher design standards and must be much more vigorously controlled during the construction process than a mixture that must meet only the moderate traffic demands and the favorable climatic conditions of another area.

In preparing the questionnaires it was assumed that in all probability the Road Test pavement, to represent national practice, would consist generally of two layers of bituminous concrete. The lower layer was referred to as the "binder course" and the upper layer as the "surface course." It may have been better not to have used the term "binder course," and to have used the terms "first course" and "second course," or "lower course" and "surface course." However, it is believed that no essential information was lost through the use of the term "binder course." While it was found that many agencies, even though using multi-course bituminous concrete, do not vary the mixture composition between courses, many others use a coarser-graded material and do not require the addition of mineral filler in the lower course or courses.

The questions that were asked in the questionnaires may be placed in two groups, one dealing with standard specification requirements, and the other dealing with general practice not outlined in detail in the specifications. This latter group of questions covered procedures that are not normally covered by specifications such as design procedures, and principal usage where specifications permit alternate usage or are sufficiently broad to allow important variations in usage.

For the purpose of the AASHO Road Test, the questionnaires were not intended to cover all details of bituminous-concrete practice, but were designed rather to obtain information where some variation in practice was believed to occur. Therefore, the reader will find that in a few instances the report may seem to underemphasize certain

important phases of bituminous-concrete construction, and in other instances over-emphasize less important phases. However, it is believed that the report will prove particularly useful to engineers already practicing bituminous-concrete construction in comparing their practices with the practices of others, and in improving their practices on the basis of the experience of others. With a proper consideration of the background for the report, the information presented should be of value also to engineers less experienced in the detailed phases of bituminous-concrete design and construction.

## BITUMINOUS-CONCRETE MATERIALS

### FINE AGGREGATE

While some of the reporting agencies distinguish between and apply separate specification requirements to the fine aggregate and the coarse aggregate to be used in bituminous concrete mixtures, others of those reporting apply requirements to only the total aggregate. For example, in the matter of gradation requirements, of the 50 reporting agencies only 20 specify gradation limits for binder-course fine aggregate, and 22 specify limits for surface-course fine aggregate; only 17 specify gradation limits for binder-course coarse aggregate, and 18 specify limits for surface-course coarse aggregate.

#### Kinds of Material

Natural sand is reported as being used as fine aggregate either optionally or exclusively by all but one of the 50 reporting highway agencies. Seven report an exclusive use of natural sand. The single agency not using sand (Delaware) permits only the use of stone screenings. Thirty-one agencies report an optional use of stone screenings, and 14 report an optional use of stone sand. Several other materials are used less extensively. Table 1-a<sup>1</sup> lists all of the materials that were reported as being used as fine aggregate in bituminous concrete mixtures, and indicates the number of agencies using each.

#### Particle Shape

Only five agencies report having specifications concerning the proportion of angular or rounded particles in the fine aggregate. The small number of agencies reporting such a requirement, and the variability of the answers that were received from them, seem to indicate that this requirement is essentially of local significance. The following descriptions were received from those answering affirmatively to the question of whether the proportion of rounded or angular particles in the fine aggregate was controlled: "fine aggregate shall consist of sand or a mixture of a minimum of 50 percent sand and a maximum of 50 percent screenings;" "specify crushed stone screenings exclusively;" "at least 50 percent passing No. 10 must be natural sand;" "fine aggregate may be 100 percent glacial sand or mixture of sand and stone screenings—50 percent maximum screenings," "not less than 50 percent or 75 percent to have one fractured face."

TABLE 1-a  
MATERIALS USED EITHER  
OPTIONALLY OR EXCLUSIVELY AS FINE AGGREGATE

Kind of Material	Number of Agencies
Natural sand	49
Stone screenings	31
Stone sand	14
Natural sand and screenings	11
Slag screenings	9
Crushed gravel screenings	8
Chat	3
Mine tailings	2
Volcanic cinders	1
Total agencies reporting	50

<sup>1</sup>The summary tables included in the text are identified by letters preceded by the number of the appendix table (Appendix 3) that contains the detailed data that have been summarized.

Three agencies not specifying the proportion of angular or rounded particles in the fine aggregate volunteered the information that the fine-aggregate material that usually is used contains from 30 to 50 percent angular particles.

### Deleterious Substances

Substances that the reporting agencies consider deleterious in fine aggregate, and the methods used to prevent the inclusion of what are considered to be harmful quantities, appear to be something of a local or regional matter and undoubtedly depend largely on experience with the aggregates at hand. Most of the reporting agencies (40 of 50) consider that their specifications recognize specifically at least one type of deleterious material. Of the 10 that do not, several report that they believe their other requirements, such as those pertaining to soundness, automatically limit the quantity of deleterious material that can be included in the fine aggregate. Others, though not volunteering the information, are undoubtedly of the same opinion.

TABLE 1-b  
LIMITATION OF DELETERIOUS MATERIALS IN FINE AGGREGATE

Material	Number of Agencies			Range of Percentage Limitations (>0)
	Specifically Limiting Material	Allowing No Amount	Having Percentage Limitation	
Clay, loam	20	11	5	0.25-15
Organic, vegetable, roots, etc.	14	11	3	0.1-1
Clay lumps	14	5	8	0.2-1
Shale	9	1	5	0.5-2 <sup>1/</sup>
Finer than No. 200 sieve; or decanted	8	0	8	1-12
Soft	6	1	3	3-5
Coal, lignite	6	0	4	0.5-1
Cemented	2	1	1	1
Other (mica, alkali, shells, cinders, salt, elongated)	5	1 <sup>2/</sup>	2 <sup>3/</sup>	0.5-1
Undifferentiated	14	11	1	3
No specific limitation	10 agencies			
Total reporting	50 agencies			

<sup>1/</sup> One state allows up to 12 percent shale in total mixture.

<sup>2/</sup> One state requires freedom from mica and salt.

<sup>3/</sup> One state allows up to 0.5 percent cinders and clinkers, and up to 1 percent mica and alkali; one state allows up to 1 percent mica.

TABLE 1-c  
SOUNDNESS REQUIREMENTS FOR FINE AGGREGATE

Test (AASHTO Standard)	Cycles	Max. Allowable Weight Loss (percent)	Number of Agencies	Remarks
Sodium sulfate	5	10	7	
	5	12	3	
	5	15	2	
	5	8	1	
	10	7	1	Stone for sand <sup>1/</sup>
	10	8	1	Natural sand <sup>1/</sup>
Magnesium sulfate	5	12	1	
	5	16	1	
	5	8	1 <sup>2/</sup>	
	10	12	1	Stone for sand <sup>1/</sup>
	10	22	1	Natural sand <sup>1/</sup>
Freeze-thaw	15	8	1 <sup>2/</sup>	
	16	25	1	Test of parent material
		Non-standard freeze-thaw	1	
Not specified			30	
Total agencies			50	

<sup>1/</sup> One agency reports four separate requirements

<sup>2/</sup> One agency reports two separate requirements

Table 1-b shows the various substances that are considered deleterious by the reporting agencies, the number of agencies that consider each as being deleterious, and the amounts of these materials that are allowed in the fine aggregate. Heading the list of materials most frequently mentioned as being deleterious are clay and loam, followed by organic materials, clay lumps, minus No. 200 or decanted, soft particles, coal and lignite, and others to a lesser extent.

Twenty of the reporting agencies place a percentage limitation on at least one specifically mentioned deleterious substance. Sixteen agencies permit the inclusion of no material that they consider to be deleterious. Two agencies place a percentage limitation on the total amount of deleterious material that may be contained in fine aggregate, without applying a specific limitation to any single substance. One agency states that the fine aggregate shall be free of an "injurious quantity of deleterious material," and another states that the quantity shall be "negligible."

Four agencies placing percentage limitations on more than one type of deleterious material place a limitation on the total that is less than the sum of the percentages for the individual types. The range of percentage limitations of this nature on the total material varies from 1.25 to 5 percent. Two agencies list more than one material as being considered deleterious, but place a percentage limitation only on the total (2 and 3 percent). Two other agencies place percentage limitations on only a portion of the individual materials that they list as being deleterious, but also place a percentage limitation (both use 5 percent) on the total.

A check of the specifications of many of the agencies limiting the quantity of "clay" and "loam" in fine aggregate indicates that few actually define these materials. It is suspected that the term "clay" usually refers to material that can be decanted, or that passes the No. 200 sieve; and that "loam" refers to topsoil of perhaps similar particle size.

### Soundness

As shown in Table 1-c, 20 agencies report having soundness requirements in their specifications for fine aggregate for bituminous-concrete construction. Thirteen base their requirements on the sodium sulfate test, and one uses the sodium sulfate test in combination with the magnesium sulfate test. Three use the magnesium sulfate test exclusively, one uses the magnesium sulfate test in combination with the freeze-thaw test, and as previously mentioned, one uses the sodium sulfate test and magnesium

sulfate test in combination. One agency bases its requirement on a freeze-thaw of the fine-aggregate parent material, and one has its own version of the freeze-thaw test.

For those agencies basing their requirements on the sodium sulfate test, at 5 cycles of testing, 7 permit up to 10 percent loss of weight, 3 permit 12 percent loss, 2 permit 15 percent, and one permits 8 percent. The three agencies reporting requirements based on the magnesium sulfate test, at 5 cycles of testing, permit 8, 12 and 16 percent weight loss respectively.

### Gradation

Twenty agencies report having gradation specifications for fine aggregate for use in binder-course mixtures. Twenty-two agencies have such specifications for fine aggregate for surface-course mixtures. All 20 of the agencies specifying gradation requirements for binder-course mixtures are among the 22 specifying fine-aggregate gradations for surface-course mixtures. Eleven of the agencies use the same fine-aggregate gradation requirements for both binder and surface mixtures.

Seven of the 20 agencies reporting gradation specifications for fine aggregate for binder-course mixtures specify percentages of material by weight passing one sieve and retained on the next. Eleven of the remainder specify percentages by weight passing a series of sieves, and two specify percentages retained. Ten agencies use the passing-and-retained basis for fine aggregate for surface-course mixtures, while 10 of the remainder specify percentages passing. Two specify percentages retained.

Not all agencies use the same separating size between fine and coarse aggregates. If it is assumed that some agencies permit as much as 10 percent oversize material to be retained on what is considered to be the nominal maximum-size sieve, (and an inspection of the data indicates that this assumption is not unreasonable, as explained later in the paper) the distribution of agencies according to nominal maximum size of fine aggregate is as follows:

Nominal Maximum Sieve Size	Number of Agencies	
	Binder-Course Fine Aggregate	Surface-Course Fine Aggregate
No. 4	11	11
No. 10	6	7
No. 8	2	3
$\frac{3}{8}$ in.	1	1
Total agencies	20	22

In order to compare the fine-aggregate gradation requirements of the reporting agencies, it was necessary that these requirements be placed on a uniform basis. The "percentage passing" basis was chosen for this particular presentation because of the ease with which the limits may be plotted for visualizing the nature of the aggregate meeting the specified requirements. A method reported in Public Roads, Volume 27, No. 7, April 1953, was used to convert "passing and retained" requirements to "percentage passing." Conversion of "percentage retained" to "percentage passing" is a common procedure of a simple nature.

After the conversion of all gradation requirements to a "percentage passing" basis, the envelope describing the upper and lower percentage limits for the various sieve combinations for each of the agencies was drawn on semi-logarithmic cross-section paper with the percentage scale on the vertical axis and the sieve sizes on the logarithmic horizontal axis. Straight lines were drawn to connect the percentage limits for the sieves in the series used by each of the agencies.

Using the envelopes that were prepared to describe the sieve-size limits of the reporting agencies, the limiting values for individual sieves were investigated. Limiting values for only the more commonly used sieves were considered in this investigation. For the agencies not having specifications based on the particular sieves chosen for study, the gradation limits that would be likely to apply were estimated from the envelope curves that had been constructed from the sieve data furnished by these agencies.


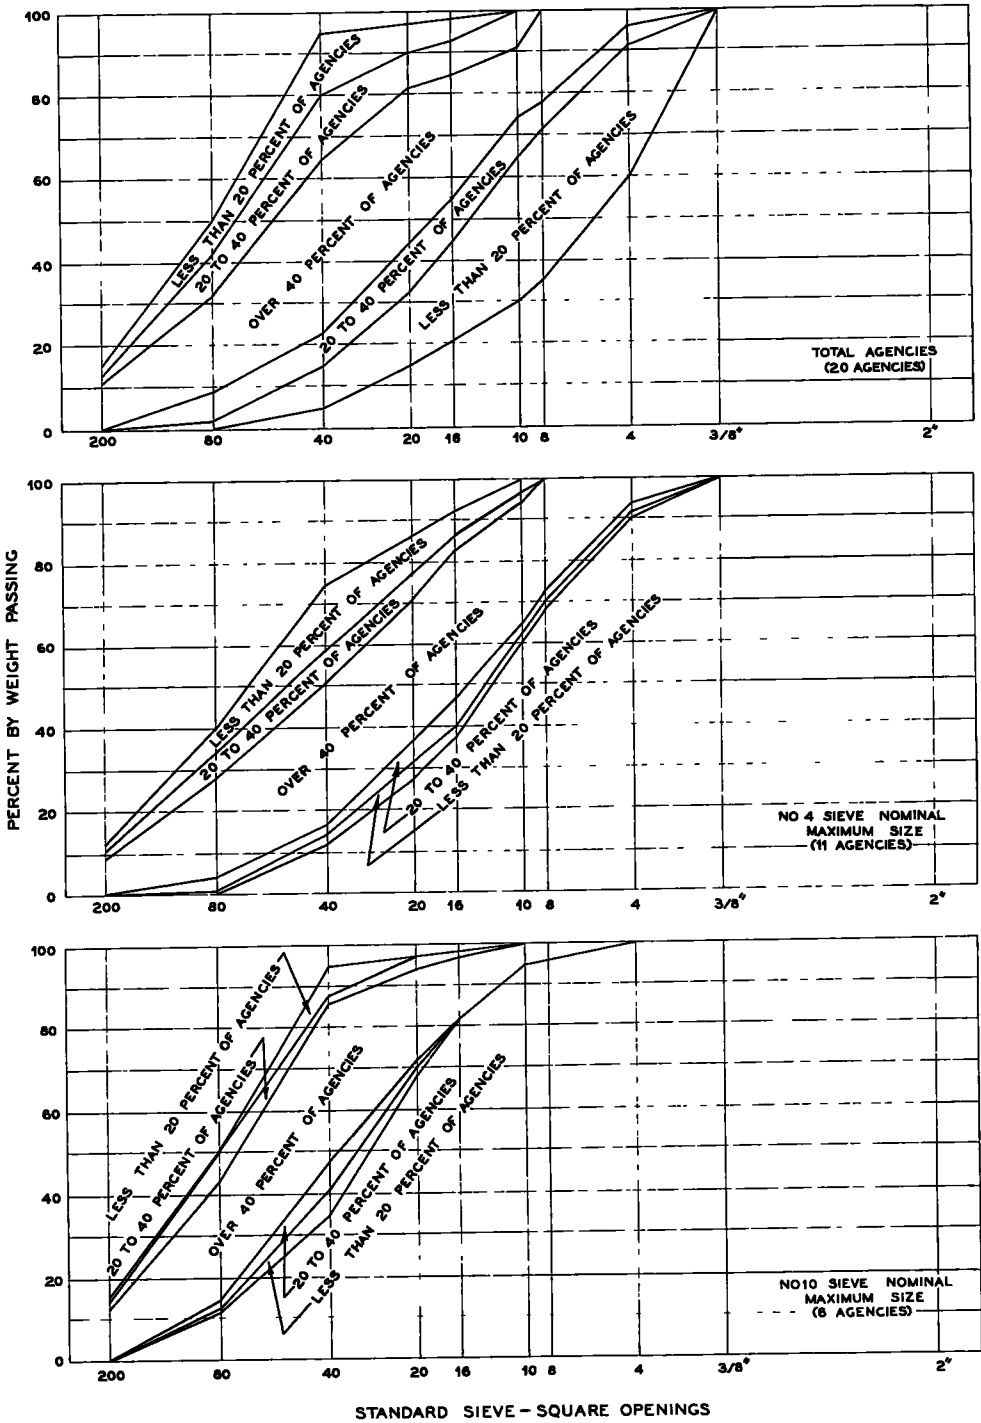


Figure 1. General acceptability with respect to gradation of fine aggregate for binder-course mixtures.

NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

For each sieve, curves of frequency of acceptance were prepared in the same manner as that employed in examining mixture gradations, as described later.

From the frequency-of-acceptance curves were determined the usage envelopes of

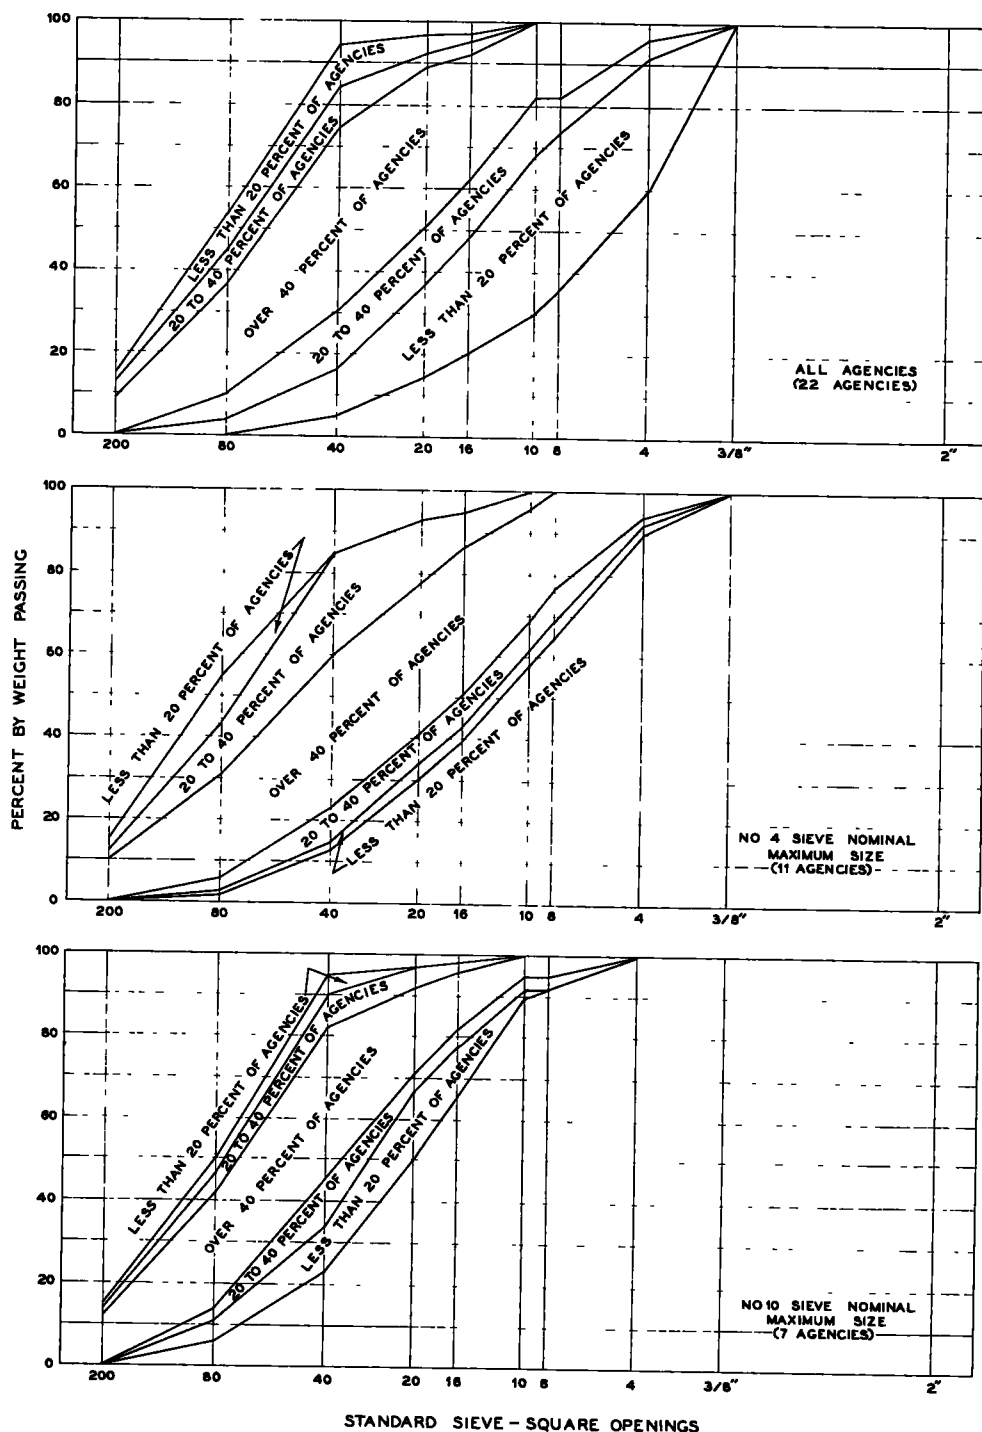

NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

Figure 2. General acceptability with respect to gradation of fine aggregate for surface-course mixtures.

Figure 1 for binder-course fine aggregate and Figure 2 for surface-course fine aggregate. The envelopes of these figures have been prepared to show: (1) limits acceptable to over 40 percent of the reporting agencies; (2) limits acceptable to 20 to 40 percent

of the reporting agencies; and (3) limits acceptable to less than 20 percent of the reporting agencies. One set of envelopes was prepared for all agencies, another set for those reporting the No. 4 sieve size as the nominal maximum size for fine aggregate, and another set for the agencies reporting the No. 10 sieve size as the nominal maximum size for fine aggregate. As would be expected, the envelopes show a much better agreement among agencies when the maximum size of material is taken into consideration.

The percentage-of-agencies separations of over 40 percent, 20 to 40 percent, and less than 20 percent were chosen arbitrarily after a visual inspection of the data indicated that such a grouping would present observable separations. This same grouping has been used also for the analysis of coarse-aggregate gradations and for the analysis of total-mixture gradations.

## COARSE AGGREGATE

### Kinds of Material

All but one of the 50 agencies replying to the questionnaires report that crushed stone is used to at least some extent as coarse aggregate for bituminous-concrete mixtures. Crushed gravel is used by 39 agencies, and crushed slag, uncrushed gravel, and other materials to a lesser extent. A complete tabulation of usage is shown in Table 2-a.

With reference to crushed and uncrushed material, 21 agencies indicate that they require all coarse aggregate to be crushed or fractured; 17 agencies permit part of the coarse aggregate to be uncrushed; and 12 agencies permit all of the coarse aggregate contained in the mixture to be uncrushed. For the 17 agencies permitting a portion of the coarse aggregate to be uncrushed, specified percentage limitations are as shown in Table 2-b.

### Wear Requirements

Wear requirements for coarse aggregates used in bituminous-concrete mixtures are specified by 48 of the 50 reporting agencies. Forty-two of these base their requirements on the Los Angeles Abrasion Test, and the remaining six use the Deval Abrasion Test. Specified maximum percentages of loss by the Los Angeles method (500 revolutions) range between 30 and 60. Nineteen agencies specify a maximum percentage loss of 40, 7 specify a maximum percentage loss of 35, and no more than 4 agencies specify any one other percentage value. A complete summary tabulation of the wear requirements for those agencies using the Los Angeles method of test appears in Table 2-c.

For the six agencies basing wear requirements on the Deval method of test, maxi-

TABLE 2-a

MATERIALS USED EITHER  
OPTIONALLY OR EXCLUSIVELY AS COARSE AGGREGATE

Kind of Material	Number of Agencies
Crushed stone	49
Crushed gravel	39
Crushed slag	18
Gravel	14
Mine chats	3
Volcanic cinders	2
Crushed boulders	1
Lava	1
Total agencies	50

TABLE 2-b

PERCENTAGE LIMITATIONS ON UNCRUSHED  
COARSE AGGREGATE PARTICLES

Maximum Percent of Uncrushed Particles Permitted in Coarse Aggregate	Number of Agencies
25	3
30	2
40	3
50	6
60	1
40 (based on total aggregate)	1
50 (based on total aggregate)	1
Total agencies	17



TABLE 2-c  
WEAR REQUIREMENTS FOR COARSE  
AGGREGATE BASED ON LOS ANGELES METHOD OF TEST

Maximum Percent Loss Allowed	Number of Agencies
60	2
55	1
50	4
48	1
45	4
40	19
37	1
35	7
32	1
30	2
Total agencies	42

mum allowable percentage loss values ranged from 3.5 to 7 for stone, and between 15 and 16 for gravel.

### Soundness

Twenty-four agencies report having a soundness requirement in their specifications concerning coarse aggregate for bituminous concrete. As will be seen from Table 2-d, most of these report basing their requirements on the AASHTO standard sodium sulfate or magnesium sulfate tests. Three use the standard freeze-thaw test, one of these in combination with the sodium sulfate test and another in combination with the magnesium sulfate test. Two agencies report using a non-standard freeze-thaw test. Twenty-one agencies report that they do not have a specific soundness requirement for the coarse aggregate, and five agencies did not reply to the question or furnished an incomplete reply.

For those agencies basing their requirements on the sodium sulfate test, at five cycles of testing, 8 agencies permit a weight loss of up to 12 percent, 3 allow a loss of up to 15 percent, 2 allow up to 10 percent, one allows up to 8 percent, and one allows up to 20 percent. For the agencies using the magnesium sulfate test, at five cycles of testing, 4 allow a loss up to 12 percent, and one allows up to an 8 percent loss.

### Deleterious Substances

As was the case with fine aggregate, the substances that are mentioned in specifications as being deleterious in coarse aggregate, and the limitations that are placed thereon are generally a matter of experience with the aggregates at hand.

Forty agencies report specific references to deleterious materials in their specifications. Nine other agencies report that they have no requirement referring directly to deleterious materials. However, some of these voluntarily stated that they believe other properties that are specified automatically limit the amount of harmful material that can be contained in the coarse aggregate. Undoubtedly others are of the same opinion.

Table 2-e summarizes information concerning the substances that are most frequently regarded as being deleterious in coarse aggregate, and indicates the range of percentage limitations that are placed on them. Organic materials, fine materials including clay and loam, clay lumps, soft particles, coal, lignite, shale, and elongated pieces are among the materials which are most frequently limited.

Twenty-two of the 37 agencies that refer specifically to one or more of the various deleterious materials (most of which are listed in Table 2-e) place a percentage limitation on at least one of them. Fourteen agencies permit no amount of material that they consider to be deleterious. Two agencies have a percentage limitation on total deleterious material without specifically limiting individual kinds, one agency states that the coarse aggregate shall be free of an "injurious quantity of deleterious material," another states that "the quantity shall be negligible," and another bases its limitations on total aggregate.

### Gradation

Insofar as gradation is concerned, the term "coarse aggregate" as applied herein

TABLE 2-d  
SOUNDNESS REQUIREMENTS FOR COARSE AGGREGATE

Test (AASHO Standard)	Cycles	Maximum Allowable Weight Loss (percent)	Number of Agencies
Sodium sulfate	5	12	8 <sub>1/</sub>
	5	15	3 <sub>1/</sub>
	5	10	2
	5	8	1
	5	20	1 <sub>2/</sub>
	10	7	1 <sub>2/</sub>
Magnesium sulfate	5	12	4
	5	8	1 <sub>3/</sub>
	10	12	1 <sub>2/</sub>
Freeze-thaw	16	10	1 <sub>1/</sub>
	50	15	1 <sub>3/</sub>
	15	8	1 <sub>3/</sub>
	Non-standard freeze-thaw		2
Not specified			21
No reply or incomplete reply			5
Total agencies			50

1/ Sodium sulfate and freeze-thaw alternate combination, one agency.

2/ Sodium sulfate and magnesium sulfate alternate combination, one agency.

3/ Magnesium sulfate and freeze-thaw alternate combination, one agency.

denotes the coarsest of a combination of two or more aggregates used to form the total aggregate portion of the bituminous concrete mixture. Two agencies reported their total aggregate gradation under coarse aggregate, but in the interest of uniformity, their reported gradations have been tabulated only as total aggregate. For the agencies listing separate gradation requirements for coarse and fine aggregates, the No. 4, No. 8 and No. 10 sieves are most frequently considered to be the separating sieves between the two sizes.

Seventeen of the 50 reporting agencies include gradation limits in their specifications for the coarse aggregate that is used in binder-course mixtures. Two of the 50 reporting agencies state that a binder course is not used, and the remainder report that they do not specify gradation limits for coarse aggregate. Eighteen agencies, including all of the 17 that specify gradation limits for binder-course coarse aggregate, specify gradation limits for surface-course coarse aggregate. Four of the 17 agencies specifying gradation limits for both binder- and surface-course coarse aggregates specify the same limits for both. The others specify generally coarser materials for use in the binder course.

TABLE 2-e  
LIMITATION OF DELETERIOUS MATERIALS IN COARSE AGGREGATE

Material	Number of Agencies		Having Percentage Limitation	Range of Percentage Limitations (>0)
	Specifically Limiting Material	Allowing No Amount		
Organic, vegetable, roots, etc.	11	7	4	0.03-1
Clay, loam	13	9	2	1
Clay lumps	18	3	15	0.05-2
Finer than No. 200 sieve; or decanted	13	0	11	0.05-4
Soft	16	1	13	2-10
Coal, lignite	9	0	8	0.25-1
Shale	16	1	11	0.5-12 <sup>1/</sup>
Elongated	10	5	4	2-15
Other (cinders, shells, schist, etc.)	7			
Undifferentiated	14	8	2	2-5
No specific limitation	9 agencies			
Total reporting	48 agencies			


<sup>1/</sup> 12 percent of total mixture

All but three of the agencies specifying coarse-aggregate gradation limits specify percentages by weight passing a series of sieves. The remaining three specify percentages retained.

Assuming that some agencies permit as much as 10 percent oversize material to be retained on what is considered to be the nominal maximum-size sieve, the distribution of agencies according to specified nominal maximum size of coarse aggregate is as shown in Table 2-f. It will be seen from the table that, on this basis, the nominal maximum size of coarse aggregate most frequently specified for binder-course mixtures are the 1-in. size (7 agencies), and the 3/4-in. size (6 agencies). For surface-course mixtures,

TABLE 2-f  
NOMINAL MAXIMUM SIZE OF COARSE AGGREGATE SPECIFIED

Nominal Maximum Sieve Size (inches)	Number of Agencies	
	Binder-Course Coarse Aggregate	Surface-Course Coarse Aggregate
1 1/2	1	
1 1/4	1	
1	7	1
7/8	1	
3/4	6	3
5/8	1	3
1/2		10
3/8		1
Total agencies	17	18

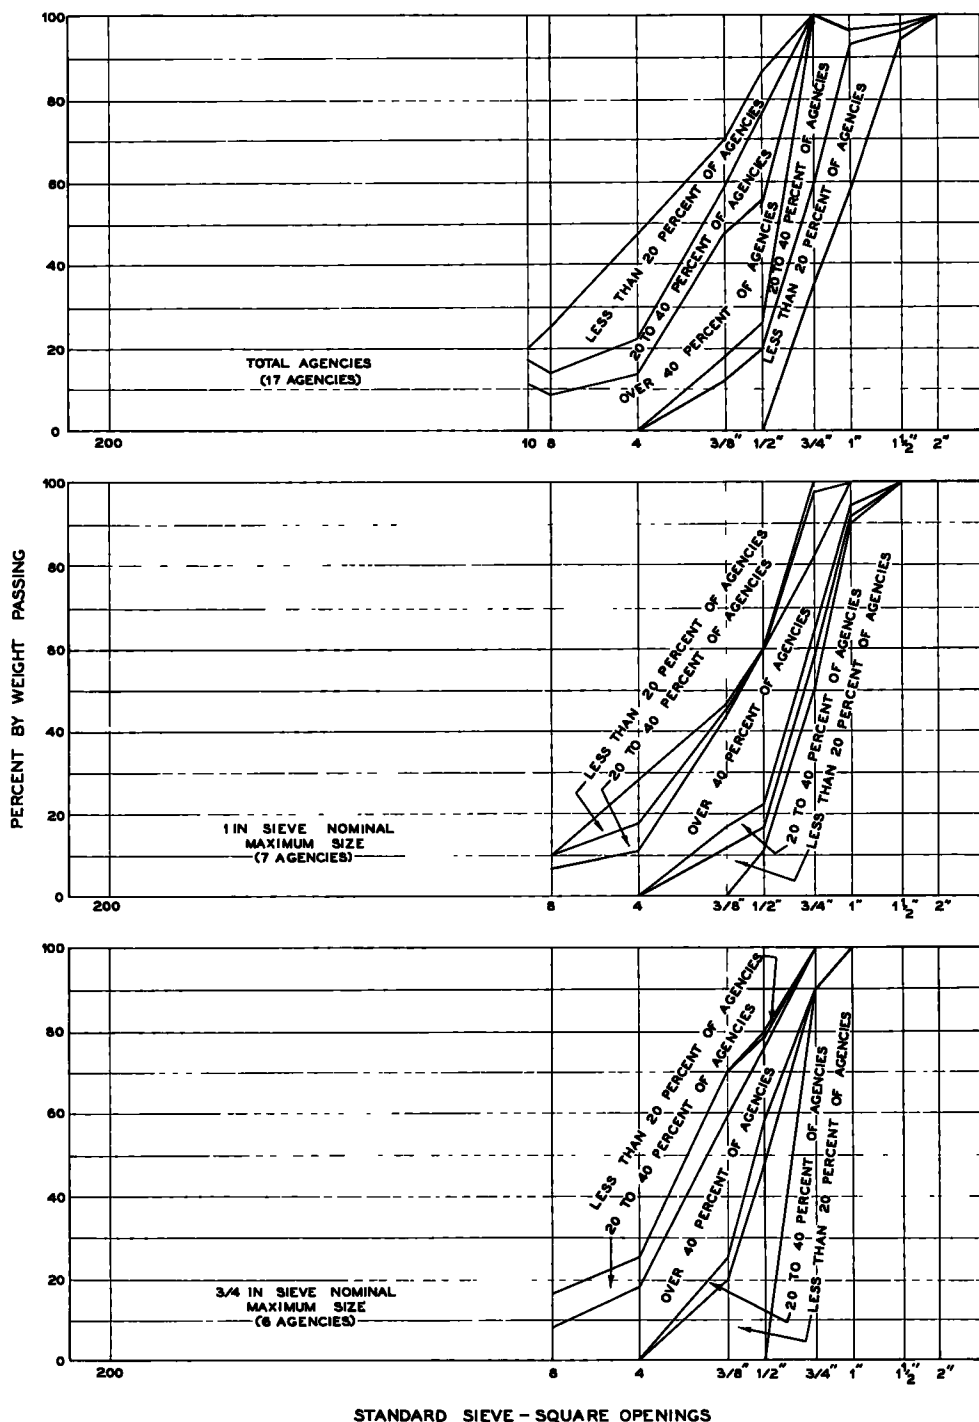


NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

Figure 3. General acceptability with respect to gradation of coarse aggregate for binder-course mixtures.

the nominal maximum sizes of coarse aggregate most frequently specified are the  $\frac{1}{2}$ -in. size (10 agencies), and the  $\frac{3}{4}$ -in. and  $\frac{5}{8}$ -in. sizes (each by 3 agencies).

Gradation-limit envelopes for the coarse aggregates were prepared in the same

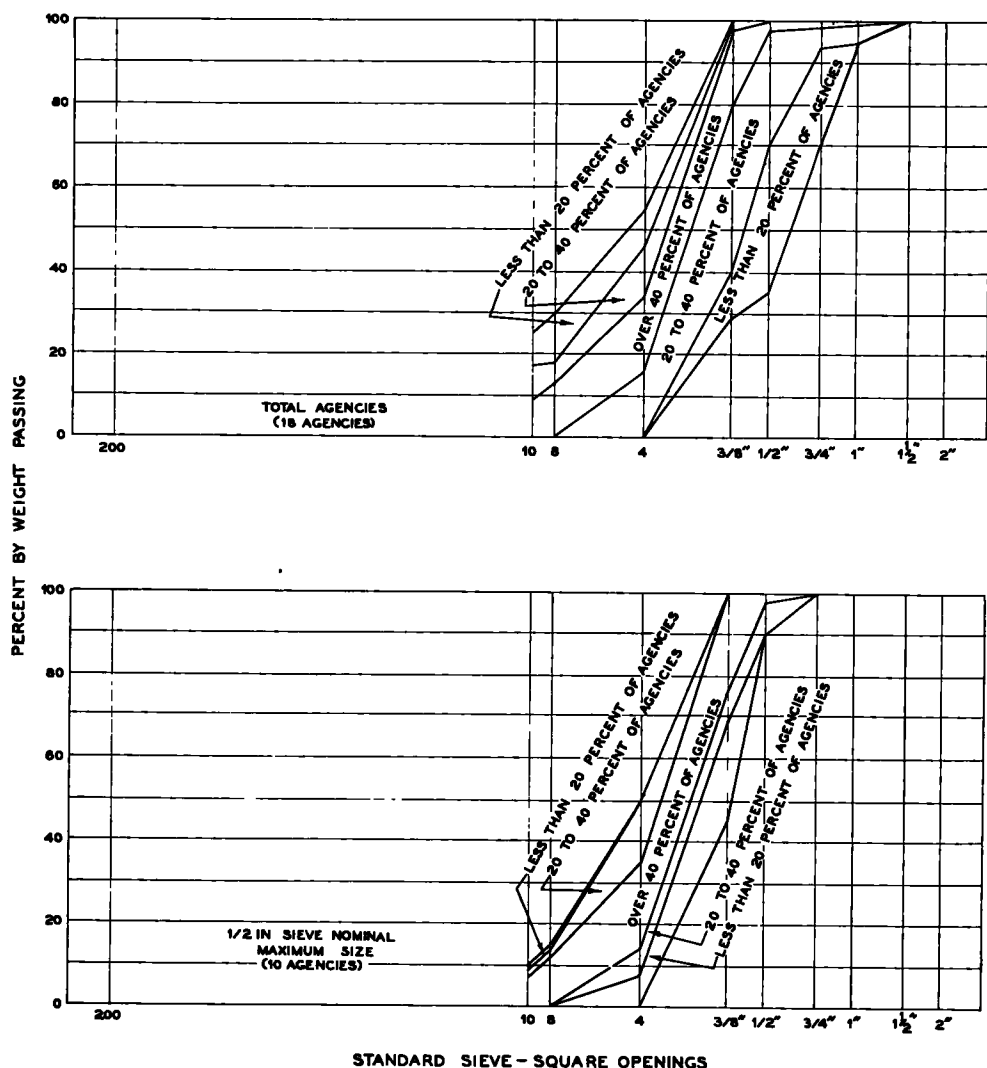

NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

Figure 4. General acceptability with respect to gradation of coarse aggregate for surface-course mixtures.

manner as that previously described for the fine aggregate. Frequency-of-acceptance curves were also prepared in the same manner as that previously described. The usage envelopes that were then developed are shown in Figure 3 for binder-course coarse aggregate and in Figure 4 for surface-course coarse aggregate. The separation of agencies into groups of less than 20 percent accepting, 20 to 40 percent accepting, and over 40 percent accepting is that which was also used for the fine aggregates and has been discussed previously.

For binder-course coarse aggregate, usage envelopes were prepared for the entire group of reporting agencies, for the agencies indicating a nominal maximum size of 1 in. for coarse aggregate, and for the agencies indicating a coarse-aggregate nominal maximum size of  $\frac{3}{4}$  in. (Fig. 3). For the surface-course coarse aggregate, usage envelopes were prepared for all of the agencies grouped together, and for the group of agencies indicating the use of a nominal maximum size of  $\frac{1}{2}$  in. for coarse aggregate (see Figure 4). It will be seen from the usage envelopes that there is a reasonably

good agreement among agencies in the matter of gradation of the coarse aggregates. The agreement is particularly good when the nominal maximum size of coarse aggregate is taken into consideration.

### Other Requirements

A few agencies listed requirements in addition to those concerning which information was specifically sought. Some of the requirements upon which information was volunteered appear to apply more directly to total aggregate rather than to coarse aggregate alone. The diversity of these miscellaneous requirements is so great as to render summarization impractical. They are listed individually in Appendix Table 2.

## MINERAL FILLER

### Kinds of Material

Forty-four of the 50 reporting agencies list one or more specific materials that their specifications permit for use as mineral filler. Though not stated specifically, the mineral-filler requirements listed by four additional agencies indicate that their filler would be soil fines or the fine fraction usually present in their granular mixtures. Two agencies state that they require no mineral filler.

The filler materials that are most frequently specified, and the number of agencies specifying them, are listed in Table 3-a. It will be noted that limestone dust and portland cement are the most frequently specified of the mineral-filler materials, followed by mineral dust, stone dust and "inert mineral matter." Seven of the agencies listing mineral dust or stone dust do not list limestone dust, so it may be presumed that their more general terms of "stone dust" and "mineral dust" would not preclude the use of limestone dust.

Other materials specifically mentioned by more than one agency as receiving use as mineral filler include hydrated lime, flyash, natural soil, basalt rock dust and shell dust. No more than four agencies mention any one of these materials.

### Gradation

Forty-three of the 50 agencies report specifying gradation limitations for the mineral filler. Fourteen of these have requirements identical to those listed in AASHTO Specification M 17-42. One of the 14 has additional requirements in the subsieve area as well. The gradation requirements of AASHTO Specification M 17-42 are as follows:

Passing No. 30 sieve	100 percent
Total passing No. 80 sieve, not less than	95 percent
Total passing No. 200 sieve, not less than	65 percent

TABLE 3-a

#### MATERIALS SPECIFIED FOR USE AS MINERAL FILLER

The gradation specifications of all but four of the remaining 29 agencies define material generally similar to that defined by the AASHTO specification. The most frequent variations from the standard specifications lie at the No. 80 and No. 200 sieves. Twenty-two of these latter agencies have either eliminated the requirements at the No. 80 sieve or have changed the requirements in such a way as to permit a somewhat greater amount of material (about 5 percent) to be retained on this sieve. Thirteen agencies have reduced the allowable amount to be retained on the No. 200 sieve by raising the lower limit on this sieve from 2 to 15

Material	Number of Agencies
Limestone dust	36
Portland cement	37
Mineral dust	11
Stone dust	10
Inert mineral matter	10
Other	12
Total agencies	44

percentage points above the AASHO specification of not less than 65 percent required to pass the No. 200 sieve.

Seven agencies, including one with the M 17-42 gradation requirement, have placed limitations on size fractions finer than the No. 200 sieve, including both sieve and sub-sieve sizes.

### Other Requirements

Only a few specified requirements in addition to those concerning the kind and gradation of material to be used as mineral filler were mentioned by the reporting agencies. A few (4) mention requirements dealing with the plasticity of the material, particularly where natural soil or the aggregate fines are considered as mineral filler. One agency specifies that the filler be non-plastic and non-hydrophilic.

## ASPHALT CEMENT

All of the reporting agencies indicate that the asphalt cements (prepared from petroleum) used in their bituminous-concrete mixtures are controlled almost entirely through the use of standard AASHO tests. The specification requirements covering the asphalt cements are also very similar or identical to those of the AASHO standard specifications (Designation: M 20-42).

TABLE 4-a

### PENETRATION GRADES OF ASPHALT CEMENT REPORTED SPECIFIED FOR BITUMINOUS-CONCRETE MIXTURES

Penetration Grade or Grades	Number of Agencies
61-70	1
60-70, 70-85	1
60-70; 70-85; 85-100	1
60-70; 85-100	4
60-70, 85-100, 100-120	1
70-85	3
70-80, 85-100	2
70-85; 85-100	3
71-80, 85-100, 150-200	1
85-100	<sup>1/</sup> 23
85-100, 100-120	2
85-120	1
85-100; 100-120, 120-150	1
85-100; 121-150	1
100-120; 120-150	1
120-150	<sup>2/</sup>
120-150, 150-200	1
150-200	1
Total agencies	50

<sup>1/</sup> Includes two agencies reporting 86-100 penetration

<sup>2/</sup> Includes one agency reporting 121-150 penetration

### Penetration Grades

The AASHO penetration grade, or the various combination of AASHO grades, reported as specified for asphalt cement for bituminous-concrete mixtures are shown in Table 4-a. The data are further summarized in Table 4-b.

Referring to Table 4-a, it will be noted that for the agencies reporting usage of a single penetration grade, far more use the 85-100 grade than any other single grade. Twenty-three agencies report the 85-100 penetration as the grade they use, while no more than three agencies indicate that usage is confined to any other single penetration grade. The lowest

TABLE 4-b

### SUMMARY OF USE OF PENETRATION GRADES OF ASPHALT CEMENT IN BITUMINOUS-CONCRETE MIXTURES

Penetration Grade	Number of Agencies
60-70 (or 61-70)	8
70-80 (or 71-80)	3
70-85	8
85-100 (or 86-100)	40
100-120	6
120-150 (or 121-150)	6
150-200	3
Total Agencies	50

grade reported used was 60-70 penetration, and the highest was 150-200 penetration.

Of the 20 agencies that consider their use of more than one penetration grade of asphalt to be sufficient to justify mention, 12 indicate that the grade selected for use is based on the anticipated traffic. Traffic was usually described as light and heavy, or light, medium and heavy. The lower penetration grades are reported to be used when traffic is expected to be heavy. Only one agency provided information in the form of definite traffic figures that determine the penetration grade to be used. This particular agency uses 70-80 penetration-grade asphalt cement where over 5,000 vehicles per day are expected, and 85-100 penetration where a lesser volume is expected.

Considering the number of agencies giving at least some usage to the various penetration grades, it will be seen from the summary of Table 4-b that more agencies make at least some use of 85-100 penetration-grade asphalt cement than of all the other grades combined.

### Total Bitumen

Thirty-three of the 50 reporting agencies require a total bitumen content (soluble in carbon disulfide) for asphalt cement of not less than 99.5 percent. This is the AASHTO standard requirement. Four agencies have a total bitumen requirement of 99.0 percent by this test, and 13 have no requirement based on this test. All of the latter group have a requirement based on the test for the proportion of bitumen soluble in carbon tetrachloride.

### Bitumen Soluble in Carbon Tetrachloride

Only 20 of the 50 reporting agencies have a requirement based on the AASHTO standard test for the proportion of bitumen soluble in carbon tetrachloride. As previously stated, 13 of these do not have a requirement based on the standard test for total bitumen (soluble in carbon disulfide). Of the 20 using the carbon tetrachloride procedure, 10 require a proportion of bitumen soluble in carbon tetrachloride of not less than 99.0 percent (the AASHTO standard), 9 require the proportion to be not less than 99.5 percent, and one agency has a requirement of not less than 99.65 percent.

### Ductility

The AASHTO standard specifications for ductility for asphalt cement require a ductility by the standard test of not less than 100 cm for grades 85-100 and higher, and of not less than the numerical value of the penetration for grades of 70-85 and lower.

All of the reporting agencies have ductility requirements based on the standard test. Of the 45 agencies listing requirements for penetration grades of asphalt of 85-100 and higher, all but two use the standard ductility requirement of not less than 100 cm. One of the latter two has a requirement of not less than 60 cm (for 85-120 penetration), and the other has a requirement of not less than 90 cm (for 85-100 penetration). Of the 14 agencies listing ductility requirements for penetration grades of 70-85 and lower, 11 show a required ductility of not less than 100 cm, only two require the ductility that is specified by the AASHTO standard, and one requires a ductility of not less than 70 for 61-70 penetration.

### Flash Point

Twenty-four of the 50 reporting agencies require a flash point of not less than 347 F, as required by the AASHTO standard specifications. The remaining 26 agencies specify higher flash points. Deviations from the standard AASHTO requirements were in some instances of

TABLE 4-c  
FLASH POINT SPECIFIED FOR ASPHALT CEMENT

Flash Point	Number of Agencies <sup>1/</sup>
Not less than 347°F. (AASHTO standard)	24
Not less than 350°F.	2
Not less than 400°F.	5
Not less than 425°F.	3
Not less than 450°F.	15
Others (ranging from 374°F. to 500°F.)	5
Total agencies	50

<sup>1/</sup> Three agencies vary flash point according to penetration grade.



TABLE 4-d

REQUIREMENTS FOR  
PENETRATION OF RESIDUE FROM EVAPORATION  
LOSS COMPARED TO PENETRATION BEFORE HEATING

Penetration Grade	Penetration Relationship (not less than, percent) $\frac{1}{2}$	Number of Agencies	AASHTO Standard Requirement
60-70 (or 61-70)	70	2	Not less than 75 percent
	75	3	
	80	1	
70-80	60	1	
	65	1	
70-85	60	1	
	70	4	
	75	3	
85-100 (or 86-100)	50	2	
	60	4	
	65	14	
	70	6	
	75	9	
	80	2	
	80.25	1	
100-120	60	2	Not less than 65 percent
	65	1	
	70	1	
	75	1	
	80.25	1	
120-150 (or 121-150)	60	1	
	65	2	
	70	2	
	80.25	1	
150-200	65	2	
Total agencies		49	

1/ Penetration of residue from evaporation loss compared to penetration before heating.

considerable magnitude. Fifteen agencies specify a flash point of not less than 450 F, and the requirements of one agency go as high as 500 F. A complete summary of general flash-point usage appears in Table 4-c.

Among the 40 agencies reporting the use of 85-100 penetration grade asphalt cement, 19 reported a flash-point requirement of not less than 347 F, and 12 report a requirement of not less than 450 F for this particular grade.

### Loss on Heating

Forty-two of the 50 reporting agencies specify the AASHO standard loss-on-heating requirement of not more than 1.0 percent. One of these agencies specifies this requirement for 85-100 penetration grade, and specifies a loss of not more than 2.0 percent for 121-150 penetration-grade asphalt. Three other agencies specify a loss on heating of not more than 2.0 percent, two specify not more than 0.75 percent, and one each specify the loss on heating to be not more than 0.2, 0.5, and 3.0 percent.

### Penetration of Residue

The AASHO standard specifications require that the penetration of residue from evaporation loss, compared to penetration before heating, be not less than 65 percent for grades of 85-100 and higher, and not less than 75 percent for grades of 70-85 and lower (using standard tests). While all but one of the reporting agencies report a specification concerning the penetration loss, the permissible values vary considerably, and departures from the AASHO standard are frequent. This will be seen from an inspection of Table 4-d where the information received concerning the requirement is summarized. Six of 16 reported requirements for penetration grades of 70-85 and lower are the AASHO standard requirement. Nineteen of 52 reported requirements for penetration grades of 85-100 and higher are the standard requirement. For agencies using requirements other than standard, the trend appears to be toward lower-than-standard percentage values where standard minimum is 75 percent, and toward higher-than-standard percentage values where standard minimum is 65 percent.

### Spot Test

The use of the spot test is listed as optional in the AASHO standard specifications (M 20-42) for asphalt cement. When specifications based on the spot test are to be included, the standard specifications require that the type of solvent to be used be stated (standard naphtha, naphtha xylene, or heptane xylene), and for the xylene solvents, the percent of xylene to be used. A negative spot condition is required under all three conditions of testing.

Thirty-six of the 49 agencies that answered the questions regarding the spot test requirements indicate that a requirement based on one of the three tests and following AASHO standard requirements is included in their specifications. Reported usage of the spot test is shown in Table 4-e. It will be noted from the table that specifications

TABLE 4-e  
ASPHALT CEMENT REQUIREMENTS BASED  
ON THE STANDARD SPOT TEST

Test	Requirement	Percent Xylene	Number of Agencies
Standard naphtha	Negative		25
Naphtha xylene	Negative	10	2
Naphtha xylene	Negative	15	3
Heptane xylene	Negative	35	6
No requirement specified			13
Not reported			1
Total agencies			50

TABLE 4-f

SPECIFIED REQUIREMENTS BASED ON TESTS OF  
ASPHALT RECOVERED FROM BITUMINOUS CONCRETE MIXTURES

Asphalt recovered by:	Agency			
	A ASTM D 762-47T	B ASTM D 762-49	C Abson Method	D 1/
Penetration, percent of original not less than	50	65	50 <sup>2/</sup> 60 <sup>3/</sup> 50 <sup>4/</sup>	65
Ductility, cm., not less than	40 <sup>4/</sup>	60 <sup>4/</sup>	50 <sup>4/</sup>	100 <sup>4/</sup>
Ash, percent, less than		1.0		
Flash point, °F., not less than				400
Loss on heating, percent, not more than				1.0
Penetration of residue from evapor- ation loss, compared to penetration before heating, percent, not less than				65
Total bitumen (soluble in carbon disulfide), percent, not less than				99.0
Spot test, naphtha xylene solvent, 15 percent xylene				Neg.

1/ Extraction by method of AASHTO T 58-30

2/ For penetration grade 75-100

3/ For penetration grades 40-75

4/ Ductility of original asphalt required to be not less than 100 cm.

are based much more frequently on the standard naphtha solvent than on the other two solvents.

#### Specific Gravity

Seven agencies report a specification requirement concerning a minimum specific gravity for asphalt cement. All but one of the other agencies answering the question concerning specific gravity (42 agencies) report having no requirement. The one additional agency with a requirement concerning specific gravity requires that there be no variations greater than plus or minus 0.02.

For the seven agencies that have a minimum specific-gravity requirement, four require that the specific gravity of the asphalt cement be at least 1.01. One of these agencies limits the 1.01 minimum to 85-100 penetration-grade asphalt, and reduces the minimum to 1.00 for 60-70 penetration-grade asphalt. One other agency has a minimum specific gravity requirement of 1.01 (85-100 penetration), another has a

minimum requirement of 1.004, (85-100 penetration) and another requires that the specific gravity lie between 1.00 and 1.04 (85-120 penetration).

An inquiry was made as to the specific gravity of the asphalt cement normally used. Forty-five of the agencies replied to this inquiry. However, the manner in which the question was worded brought a variety of answers that were not subject to precise summarization. Generally speaking, the replies appear to indicate that most of the asphalts being used have specific gravities between 1.00 and 1.03. A specific gravity of about 1.02 appears to be an approximate central value. Only two or three agencies indicate that their specific gravities fall below 1.00 (a low of 0.98 was reported), and only nine agencies report values higher than 1.03 (with a top of 1.05).

### Recovered Asphalt

Four agencies report that they have set up specification requirements based on tests of asphalts recovered from bituminous-concrete mixtures. Two of these agencies indicate that the asphalt is recovered by the Modified Abson Method of ASTM D 762 (one stated, D 762-49, and the other D 762-47T), and one agency simply reports using the "Abson Method." The fourth agency indicates that extraction is made by the method of AASHTO T 58-30, but does not indicate the method of recovery.

The tests that are conducted on the recovered asphalt, and the specified limiting values placed on the characteristics measured by the four agencies, are shown in Table 4-f. It appears that the most important of the tests are the penetration and ductility tests. For the four agencies reporting, the penetration of the recovered asphalt is not permitted to be less than from 50 to 65 percent of the penetration of the asphalt as originally tested. Three of the agencies indicate that they will permit the ductility to fall to from 40 to 60 cm (the ductility requirement for the original material being not less than 100 cm). The fourth agency requires the ductility value to be not less than 100 cm both before and after recovery.

The questions that were asked regarding the general practice in recovering and testing recovered asphalt were unfortunately not well worded, and the tabulations may not entirely reflect actual practice. For example, it was asked: "Do you regularly measure the characteristics of recovered asphalt from bituminous mixture samples?" Seven agencies replied affirmatively, and ten, though indicating that they did not test recovered asphalt regularly, volunteered the information that they did do a limited amount of testing. Thirty-one agencies replied negatively to the question, but volunteered no information as to whether a limited amount of testing is done. It is suspected that there are among the 31 several that do a limited amount of testing of the characteristics of recovered asphalt.

The question concerning the method used to extract and recover the asphalt from bituminous-concrete mixtures was apparently equally confusing. Eighteen agencies referred to ASTM Designation D 762, four referred to ASTM Designation D 1097 (two of these referring to D 762 also), and 15 referred to AASHTO Designation T 58 (with four of these stating that the test was used for extraction only). Other methods mentioned, none by more than one or two agencies, were the Abson, the Oliensis, the Bessow, and modifications of ASTM D 762 and AASHTO T 58. It appears from the answers that some of the agencies, though not so stating, intended their answers to refer only to extraction methods.

### Other Specification Requirements

A few agencies volunteered information on asphalt-cement requirements in addition to those previously discussed. Several mentioned the requirement contained in the AASHTO standard specifications to the effect that the asphalt shall be free of foam when heated to 347 F. Others undoubtedly have the same requirement but did not furnish the information since no specific question was asked concerning this requirement. Five agencies reported a softening point requirement. One agency reported a requirement that the ductility at 39.2 F shall not be less than 10 percent of the penetration, and another reported a requirement that the ductility at 39.2 F shall not be less than 30 percent of the penetration value.

In answer to the question of whether the thin-film oven test was required by specification, all agencies answered in the negative.

### COMPOSITION OF BITUMINOUS-CONCRETE MIXTURES

All of the agencies that replied to the questionnaires (50) indicate that they use mixtures of a composition that they term "bituminous concrete." One agency reports that it confines its use of bituminous concrete to the surface course only. Three agencies indicate that their composition limits for binder-course and surface-course mixtures are the same. There appears to be reasonable agreement among agencies as to the sort of a mixture that should be termed "bituminous concrete." In general, the prescribed gradation limits provide for a mineral aggregate that is continuously graded from coarse to fine. All of the agencies use asphalt cement, though of various penetrations, as the binding medium. The reported asphalt-cement contents of the mixtures do not differ widely.

#### Gradation of Mineral Aggregate

Specifications outlining the general limits of particle-size distribution are expressed in one of three forms: (1) maximum and minimum percents by weight of material to pass each of a given series of sieves; (2) maximum and minimum percents by weight of material to be retained on each of a given series of sieves; and (3) maximum and minimum percents by weight of material to pass each and to be retained on the next finer of a series of sieves. For binder-course material, 48 agencies reporting, 33 use the percent-passing method, 12 use the passing-and-retained method, and 3 use the percent-retained method. For surface-course material, 50 agencies reporting, 32 use the percent-passing method, 15 use the passing-and-retained method, and 3 use the percent-retained method.

All of the agencies that specify the sieve gradation limits for aggregate for mixtures on a "percent passing" or "percent retained" basis base the percentage requirements on the total weight of aggregate. With two exceptions, the agencies that specify the sieve gradation limits on a "passing-and-retained" basis base the aggregate percentage requirements on the total weight of the mixture, inclusive of the bitumen. The other two use the total-aggregate basis.

All but five of the reporting agencies specify the bitumen content of mixtures as a percentage of the total mixture. The remaining five, all of which use either the "percent-passing" or "percent-retained" methods in specifying the aggregate, specify the bitumen content of mixtures as a percentage of the total aggregate.

Any of the three methods is satisfactory for outlining the general limits of gradation for mineral aggregates. The range between the maximum and minimum limits for any sieve, or between consecutive sieves if the passing-and-retained method is used, can be broadened or narrowed depending on the general range of gradations that, if met, will produce a satisfactory mix.

The degree of general control is further influenced by the number of sieves that are used to specify the grading of the aggregate. The greater the number of sieves, the greater will be the degree of control that can be exercised over the material through the entire range of gradation. For the reporting agencies, 12 use a total of 7 sieves to specify binder-course materials, and 24 use 7 sieves to specify surface-course materials. Other numbers of sieves used with considerable frequency for specifying binder-course materials are 9 (by 8 agencies), and 5 (by 7 agencies). Twelve agencies use 8 sieves for specifying surface-course materials. The number of sieves reported in use for specifying binder-course materials ranged from 2 to 13, and for surface course mixtures from 3 to 10.

For surface-course mixtures, a small amount of mineral dust passing a No. 200 sieve is almost always required. Only two of 49 agencies reporting requirements on the No. 200 sieve for their highest type of asphaltic-concrete surface-course mixtures indicate that a mixture with no particles passing the No. 200 sieve would be acceptable. One agency does not include in its specifications a sieve finer than the No. 100. However, this agency requires a certain amount of the material to pass the No. 100 sieve.

For binder-course mixtures, a small amount of dust passing the No. 200 sieve is always permitted, but not always required. Twenty-four of 48 agencies reporting on binder-course requirements do specify that a small amount of material must pass the No. 200 sieve.

Considerable variation occurs in the maximum size of the mineral aggregate that is permitted in asphaltic concrete by the reporting agencies. As would be expected, most of the agencies use a smaller size aggregate in surface-course mixtures than in binder-course mixtures. Usage with respect to the maximum size of aggregate is shown

TABLE 5-6-a

FREQUENCY OF USE OF VARIOUS MAXIMUM SIZES  
FOR MINERAL AGGREGATE

Sieve Size (inches)	100 Percent to Pass <sup>1/</sup>	Number of Agencies	
		95 Percent or More to Pass	90 Percent or More to Pass
<u>Binder-Course Aggregate</u> (48 agencies)			
2	2	-	-
1 3/4	1	2	1
1 1/2	5	4	5
1 1/4	12	9	2
1	14	13	16
7/8	2	2	2
3/4	10	15	18
5/8	1	1	1
1/2	1	2	3
<u>Surface-Course Aggregate</u> (50 agencies)			
1 1/4	2	-	-
1	11	6	4
3/4	13	14	13
5/8	4	4	4
1/2	20	24	26
3/8	-	2	3

<sup>1/</sup> Agencies not stating a 100-percent-passing requirement are placed in the sieve-opening group next above the maximum size listed in specifications.

in Table 5-6-a. For the purpose of this discussion, three separate groupings are shown in the table. The first grouping is based on the maximum size of sieve that all aggregate is required to pass. For those agencies that do not set a top size that all material must pass, the next largest standard sieve size above the top size mentioned in their specifications is assumed as the sieve through which all material must pass. As an example, an agency requiring that 95-100 percent of aggregate must pass a 1-in. sieve, but having no requirement based on a sieve with larger openings, would be placed in the  $1\frac{1}{4}$ -in. top-size group. The second grouping is based on the assumption that any agency specifying that at least 95 percent pass a sieve, but accepting up to 100 percent passing considers that sieve opening to be the nominal top size of the material they use, and permits up to 5 percent oversize material. The third grouping is similar to the second grouping except that the assumption is made that any agency requiring at least 90 percent to pass a specified sieve, but accepting up to 100 percent passing the sieve, considers the openings of that particular sieve to be the nominal top size of the aggregate. It will be noted from Table 5-6-a that, for binder-course materials, the most frequently specified top sizes by the first method of grouping are the  $1\frac{1}{4}$ -in., 1-in., and  $\frac{3}{4}$ -in. sizes. For the second and third methods of grouping, the 1-in. and  $\frac{3}{4}$ -in. sizes predominate. For surface course mixtures, the  $\frac{3}{4}$ -in. and  $\frac{1}{2}$ -in. top sizes predominate regardless of the method of grouping, although by the first method of grouping a considerable number of agencies are also shown to use a 1-in. size group.

As was indicated earlier in the report in the sections concerning the fine and coarse aggregates, the comparisons involving the maximum size of aggregate that are made in the gradation analyses in this report are made with the assumption that the nominal maximum size is the sieve size through which at least 90 percent of the material is required to pass, but through which up to 100 percent is allowed to pass. In other words, it is assumed that some agencies are specifying that material containing up to 10 percent of particles larger than the nominal size is acceptable. This assumption is not based on specific information that was received from the reporting agencies. However, grouping of gradation limits based on this assumption provided the best showing of uniformity of practice among agencies.

The size of the mineral-aggregate particles and the distribution of sizes from coarse to fine are recognized by all to have an important bearing on the performance of bituminous concrete. A continuous grading in sizes of particles from coarse to fine, with no great concentration at any one particle size and with no absence of particles at any size, is generally considered productive of the best bituminous concrete. Because of the influence of angularity, roundness, and probably other considerations, there is apparently no ideal gradation that is suitable for all aggregates. And if there were, practical considerations would require that a certain amount of deviation from the ideal be permitted to keep costs within reason.

Each agency exercises a control of gradation and uniformity that it considers consistent with its needs and ability to financially fulfill these needs. This brings about a certain amount of variation in the degree of control that is exercised over the gradation of the mineral aggregate.

All of the reporting agencies include in their general specifications prescribed sieve-size limits for the mineral aggregates to be contained in bituminous-concrete surface-course mixtures. All but one of the agencies using bituminous-concrete binder-course mixtures include prescribed sieve-size gradation limits for the binder-course aggregate in their general specifications. The single exception reports that special provisions regarding sieve-size limits are written to fit aggregates available in the area of construction projects where the binder-course mixture is to be used.

Besides controlling the gradation of the mineral aggregate, it is considered desirable by most agencies to also control the uniformity of grading of the aggregate from coarse to fine. Two different methods are generally used to accomplish this purpose. The first of these is to use the passing-and-retained method of specifying gradation limits. By this method considerable assurance is offered that there will not be an excess or deficiency of particles between successive sieves. As stated previously, 12 agencies use the passing-and-retained method of specifying mineral aggregate for binder-course mixtures, and 15 use the passing-and-retained method for surface-

course mixtures. One of these agencies requires, in addition, a prescribed total percentage of material to pass the No. 10 sieve for both binder- and surface-course mixtures. Another requires a prescribed percentage to pass a No. 6 sieve for surface-course mixtures.

For the agencies specifying gradation limits by the percent-passing method, a few (six) attain increased uniformity by specifying a certain minimum percentage of material to be retained between successive sieves. Four of these require that at least four percent of the material be retained between successive sieves. The other two require that at least five percent be retained between successive sieves smaller than the  $\frac{3}{8}$ -in. sieve.

Additional uniformity obtained through the use of job-mix formulas and tolerated variations therefrom will be discussed later.

Of considerable interest is comparison of the gradations of the mineral aggregates specified by the reporting agencies. To make such a comparison, it is first necessary to place all of the prescribed gradations on a common basis. As explained earlier in the report the percent-passing basis has been chosen for making this comparison because of the more common use of this method, and also because of the greater ease with which gradations prescribed by this method may be plotted for visual examination. As is usually done, charts on semilogarithmic paper with a percentage scale on the vertical axis and the sieve sizes in logarithmic scale on the horizontal axis have been used for the comparisons.

Percent-retained limits were converted to percent-passing limits by simple sub-

TABLE 5-b  
SIEVE-SIZE GRADATION LIMITS FOR ALL AGENCIES  
CONVERTED TO COMMON BASIS - BINDER-COURSE MIXTURES

Agency	Indicated Limiting Percentages by Weight of Total Aggregate Permitted to Pass Sieve																
	2 in	1 3/4 in	1 1/2 in	1 1/4 in	1 in	7/8 in	3/4 in	5/8 in	1/2 in	3/8 in	No. 4	No. 10	No. 20	No. 40	No. 60	No. 100	
Ala					100		75-100		55-95	47-77	35-77	24-50	17-30	12-30	4-15	0-5	
Ariz							Variable										
Ark					100		0-95		0-100	54-74	40-75	27-40	17-30	10-25	5-15	0-5	
Calif					100		95-100		75-100	0-75	40-75	27-40	17-30	11-19	7-13	3-5	
Colo					100		90-100		75-90	0-100	50-100	25-40	17-30	10-25	5-15	0-5	
Conn					100		90-100		75-90	0-100	50-100	25-40	17-30	10-25	5-15	0-5	
Del					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
D C					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Fla					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Ga					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Idaho					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Ill					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Ind					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Iowa					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Kans					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Ky					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
La					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Maine					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Mass					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Mich					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Minn					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Miss					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Mo					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Mont					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Nebr					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Nev					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.J.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.H.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.Y.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.C.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.Dak					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.I.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
N.Mex					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Okla					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Oreg					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Penn					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
R.I.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
S.Dak					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
S.C.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
S.D.					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Tenn					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Tex					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Utah					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Vt					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Wa					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Wash					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
W.Va					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Wis					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Wy					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	
Ontario					100		90-100		70-100	50-100	40-55	25-45	17-30	10-25	5-15	0-5	



TABLE 6-b

SIEVE-SIZE GRADATION LIMITS FOR ALL AGENCIES CONVERTED  
TO COMMON BASIS - SURFACE-COURSE MIXTURES

Agency	Indicated Limiting Percentages By Weight of Total Aggregate Permitted to Pass Sieve											
	1 1/4 in.	1 in.	3/4 in.	5/8 in.	1/2 in.	3/8 in.	No. 4	No. 10	No. 20	No. 40	No. 80	No. 200
Ala.		100	95-100		75-88	60-80	40-60	20-40	14-32	10-25	5-15	2-8
Ariz.		100	85-90		62-80	45-65	37-57	25-45	19-34	15-25	8-17	2-10
Ark.			100		87-100	77-88	55-75	40-55	26-41	15-30	9-20	4-10
Calif.		100	95-100		75-85	60-75	40-55	28-38	17-26	11-19	7-13	3-6
Colo.		100	90-100		70-85	61-75	40-52	29-38	24-33	19-27	13-21	4-8
Conn.	100	95-100	82-100		60-100	51-86	28-55	22-44	17-37	12-31	8-18	4-8
Del.				100	91-100	80-100	50-65	30-45	20-30	15-25	10-20	5-10
D. C.					100	80-100	55-80	40-75	23-50	10-30	3-15	2-8
Fla.					100	61-92	33-84	24-75	22-63	19-53	10-26	5-8
Ga.					100	95-100	50-80	44-61	30-46	20-38	11-23	5-10
Idaho				100	88-100	72-87	45-65	30-50	24-40	18-32	12-22	5-12
Ill.			100		95-100	78-92	42-73	27-62	25-57	22-46	15-23	4-9
Ind.					100	85-98	32-76	21-72	14-54	8-40	4-18	3-9
Iowa		100	98-100		80-92	67-87	47-61	34-53	23-40	17-30	8-20	3-10
Kans.		100	95-100		78-93	65-88	53-77	37-61	24-43	17-29	11-15	6-12
Ky.					100	85-100	50-70	31-48	15-34	6-24	1-12	0-5
La.			100		85-100	78-95	60-80	40-60	29-51	20-35	12-25	4-10
Maine					100	80-100	35-75	30-55	24-45	12-40	7-19	3-8
Md.		100	88-100		76-88	66-80	48-62	32-44	18-31	10-20	6-14	2-8
Mass.					100	87-100	58-73	31-57	21-52	15-34	9-17	4-6
Mich.				100	93-100	83-100	61-76	32-47	25-37	19-28	12-19	5-9
Minn.			100	98-100	87-93	70-85	50-65	35-50	24-38	15-30	8-16	4-3
Miss.					100	95-100	80-95	55-75	40-57	28-42	12-24	6-10
Mo.			100		97-100	71-100	29-78	22-71	18-60	15-52	9-30	4-11
Mont.			100		76-100	58-84	34-73	25-64	19-54	15-47	9-25	4-9
Nebr.		100	96-100		81-97	70-95	45-65	25-45	19-34	14-26	8-17	5-10
Nev.	100	95-100	81-92		60-80	52-69	37-51	28-38	24-32	20-27	13-20	5-11
N. H.					100	80-95	45-75	30-50	17-37	10-30	5-20	3-8
N. J.			100		85-100	74-100	26-78	19-73	18-67	14-54	7-26	4-9
N. Mex.			100		90-100	55-85	40-65	30-50	22-38	15-30	8-20	4-10
N. Y.		100	98-100		95-100	82-93	46-74	17-52	8-34	6-24	3-13	2-6
N. C.			100		95-100	79-90	42-68	22-57	17-50	14-44	6-22	2-9
N. Dak.			100		82-100	68-93	44-78	25-60	18-47	13-34	7-20	2-8
Ohio		100	95-100		74-93	43-86	24-75	23-67	13-47	7-30	2-16	0-5
Okla.			100		90-100	79-94	55-80	40-55	29-44	20-37	10-25	4-8
Oreg.			100		85-100	73-88	48-60	27-43	17-32	9-23	6-14	3-7
Pa.					100	80-100	45-72	28-52	16-34	9-24	3-13	2-8
R. I.					100	84-100	28-73	27-72	19-56	12-34	9-17	5-9
S. C.					100	75-97	58-75	42-60	36-52	25-35	15-25	5-12
S. Dak.		100	90-100		75-90	64-83	47-70	35-55	27-41	20-30	13-20	6-10
Tenn.					100	89-100	64-76	46-56	31-40	19-27	7-14	3-8
Tex.				100	97-100	75-88	37-69	12-57	12-57	7-38	2-11	
Utah					100	90-100	70-100	60-90	43-79	30-70	10-40	5-12
Vt.					100	61-92	46-84	24-75	22-63	19-53	10-26	5-8
Va.					100	80-100	50-70	35-50	21-36	10-25	3-15	2-10
Wash.				100	90-100	69-87	35-62	20-40	15-33	10-28	3-18	1-6
W. Va.					100	85-100	60-80	37-57	21-38	11-26	5-14	1-5
Wis.			100		95-100	75-100	45-85	30-55	22-44	15-35	10-25	5-12
Wyo.					100	84-100	50-70	30-50	23-39	18-31	12-20	5-10
Ontario					100	75-88	50-60	37-58	23-48	16-34	7-15	3-8

traction. Passing-and-retained limits were converted to percent-passing limits by the method described in the article "Plotting Aggregate Gradation Specifications for Bituminous Concrete," (Public Roads, April 1953).

In instances where the specified percentages are based on the total mixture, these were converted to percentage limits based on the total aggregate. All but two of the agencies using the passing-and-retained method of specifying the mineral aggregate base the gradation limits on the total mixture. All other agencies base the percentage limits on the total aggregate.

Two agencies base their specifications on sieves with round openings for sizes of 1/4-in. and greater. All of the other agencies use sieves with square openings. The


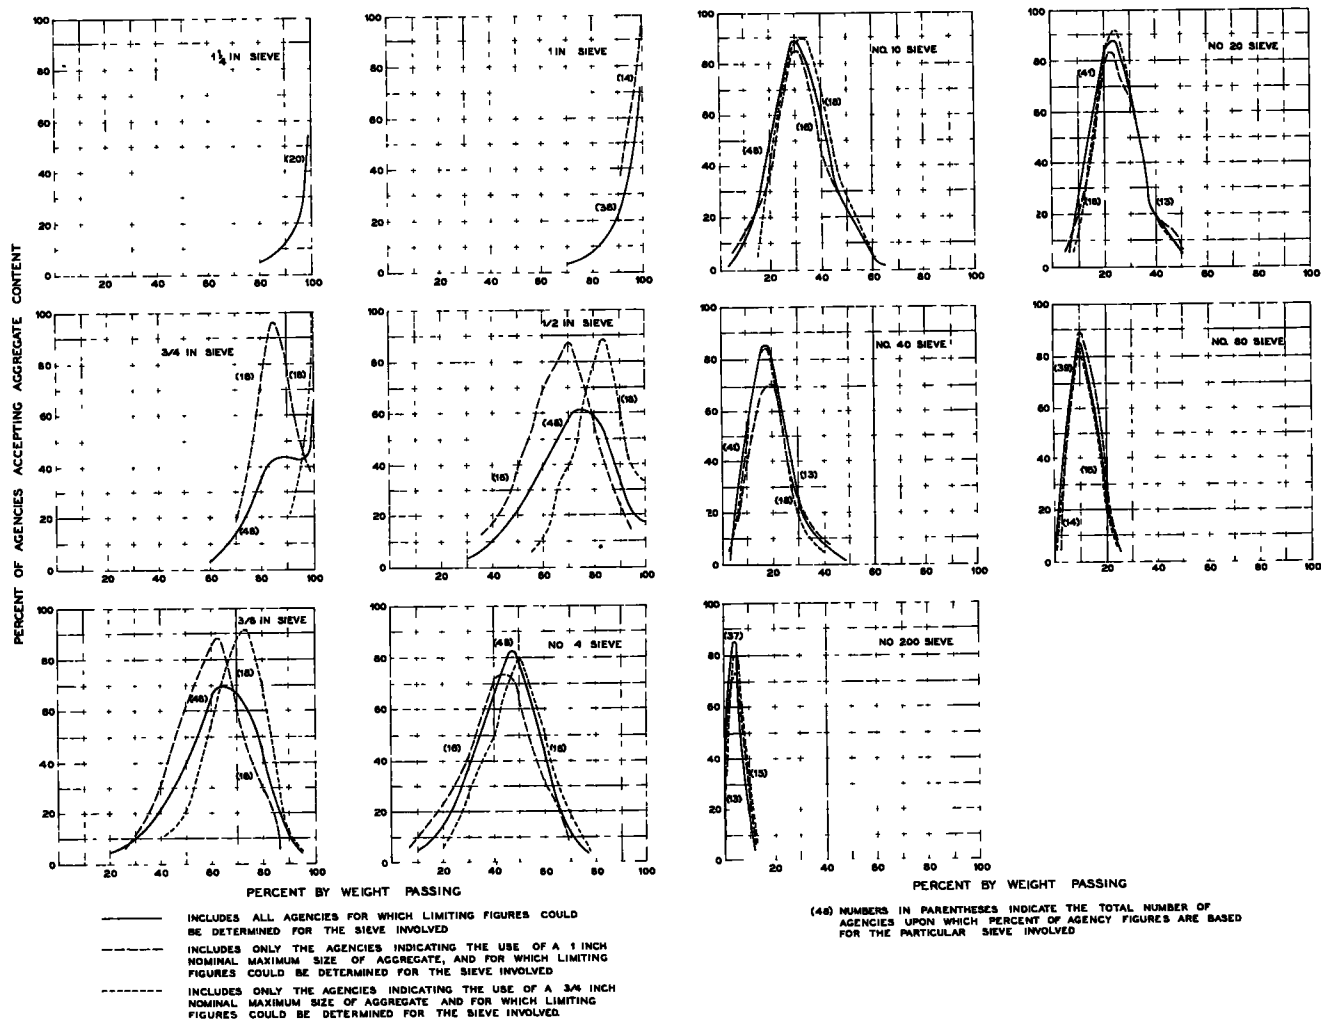


Figure 5. Frequency of acceptance of percentages of aggregate passing various sieves - binder-course mixtures.

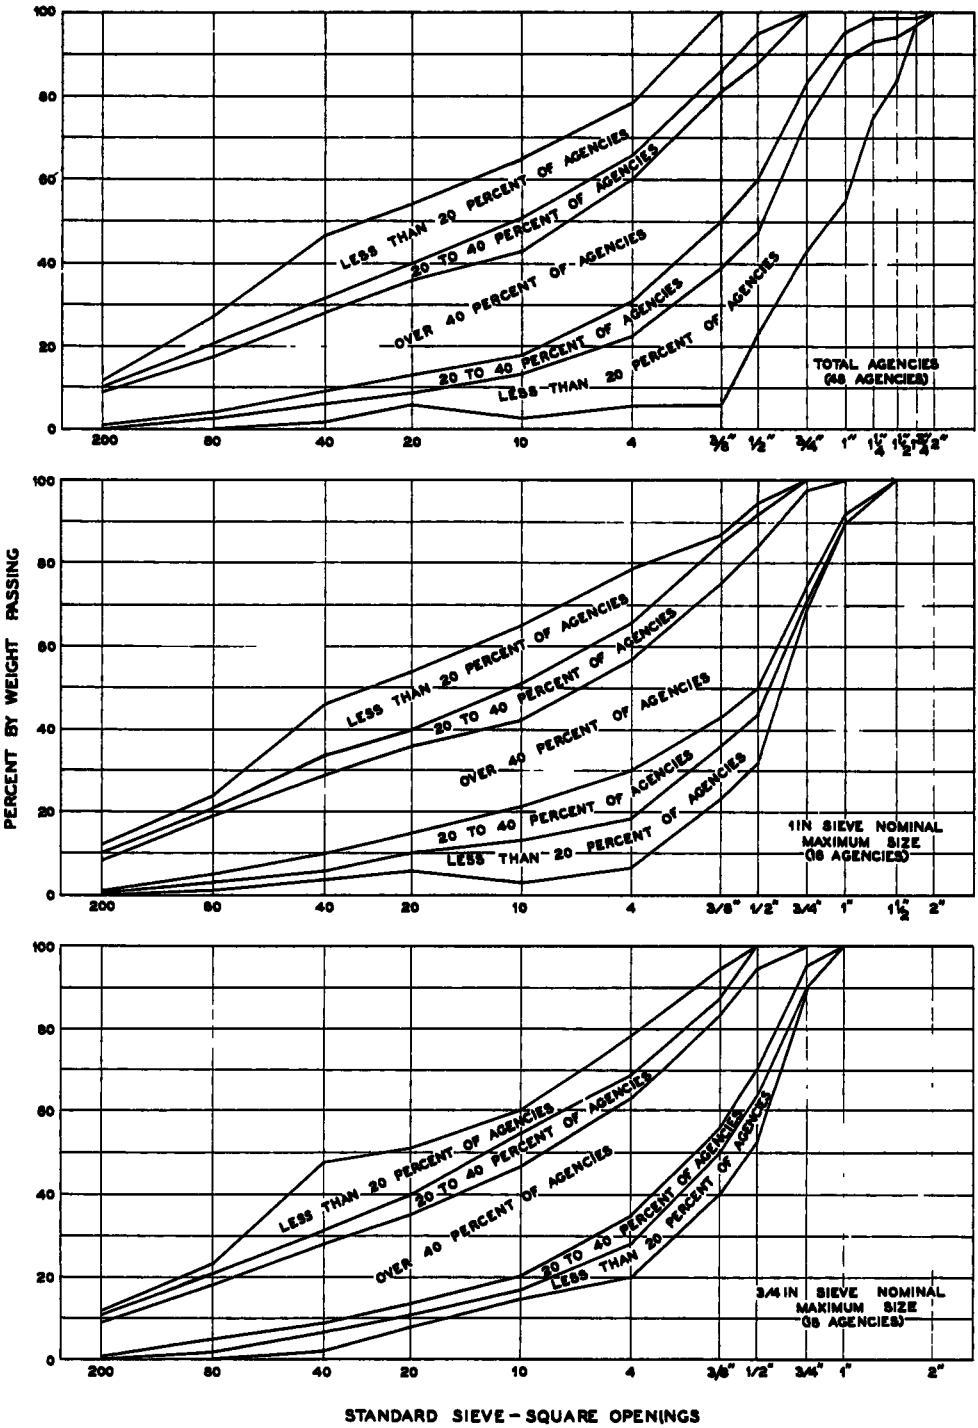

NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

Figure 6. General acceptability with respect to gradation of total aggregate for binder-course mixtures.

requirements of the two agencies using the round openings were converted to square openings on the basis of the following table which was found in the New Jersey specifications:

### Conversion from Round to Square Openings

Round Openings	3½ in.	3 in.	2¼ in.	1¾ in.	¾ in.	½ in.	¼ in.	10	30	200
Square Openings	3 in.	2½ in.	1⅞ in.	1 in.	⅝ in.	⅜ in.	No. 4	10	30	200

Following the conversion of all gradation specification limits to a common basis, the limits of each agency were plotted on semilogarithmic paper to form the familiar gradation envelope. The envelopes were formed by connecting the plotted points with straight lines. In instances where agencies did not specify a maximum size, the lower line of the envelope was extended to the 100-percent point on the next commonly-used sieve above that which is specified by the agency. In a few instances where a 100-percent-passing figure was listed, followed by specified limits on a much smaller sieve, an unrealistically narrow upper portion of the envelope would result if the upper boundary of the envelope were formed by connecting the 100-percent point to the upper-limit point for the first sieve listed below the top-size sieve. In these few cases this


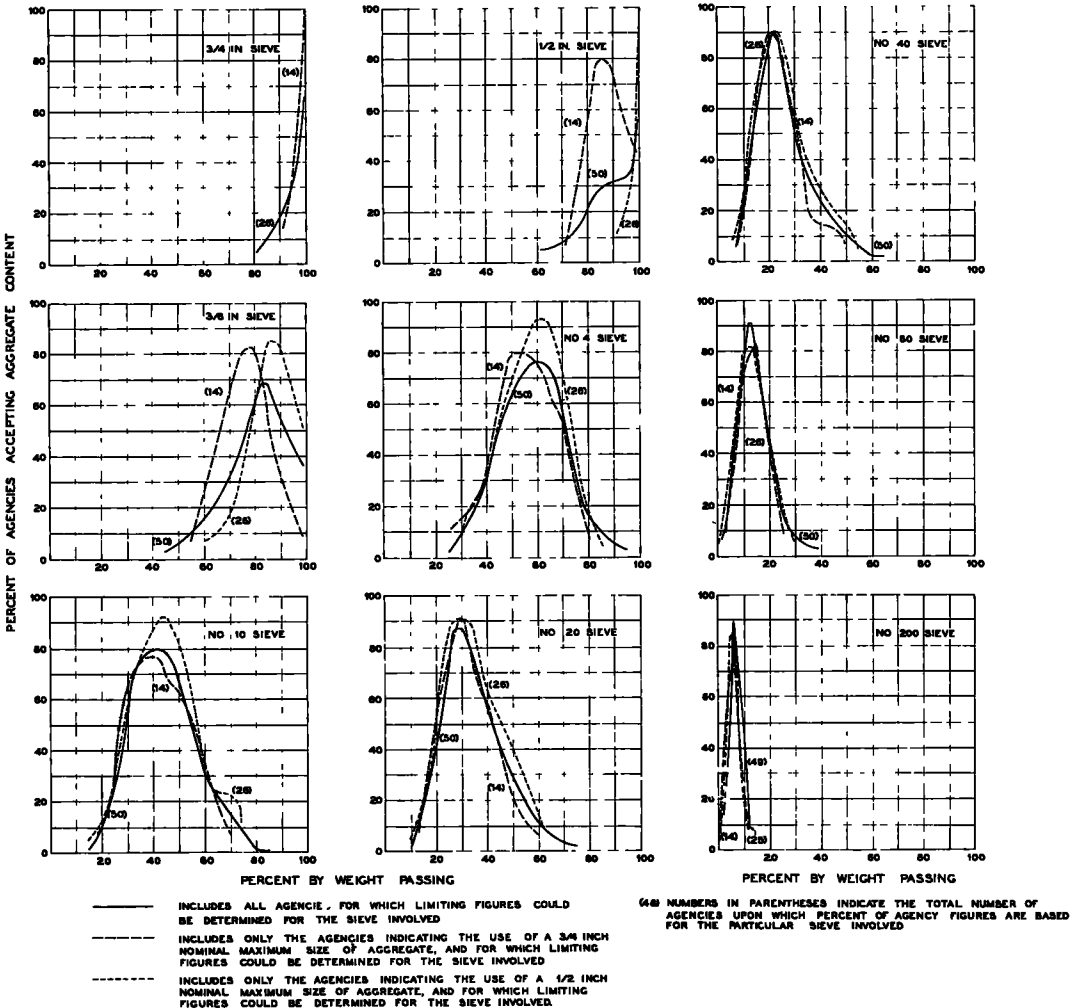


Figure 7. Frequency of acceptance of percentages of aggregate passing various sieves - surface-course mixtures.

portion of the envelope was determined by arbitrarily drawing the line to the 100-per-cent point on a sieve one or two sizes smaller than the maximum specified.


After all envelopes had been plotted, the percentage values were determined for all

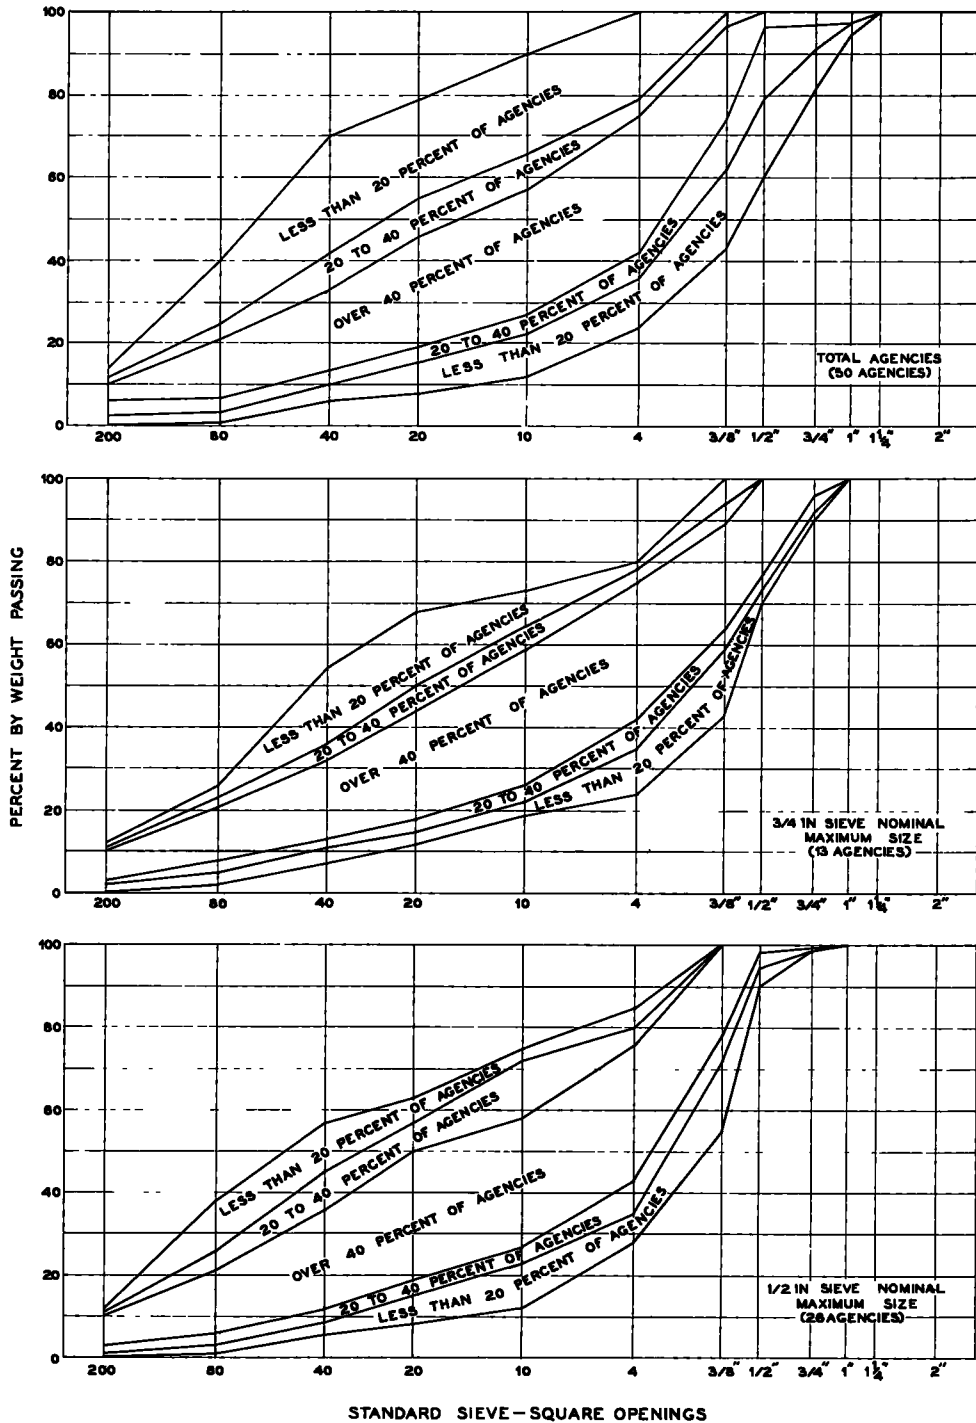


NOTE FOR THE PURPOSE OF THIS PRESENTATION, THE NOMINAL MAXIMUM SIZE IS ASSUMED TO BE THE SIZE OF THE SIEVE ON WHICH NOT MORE THAN 10 PERCENT IS ALLOWED TO BE RETAINED, BUT THROUGH WHICH 100 PERCENT MAY PASS

Figure 8. General acceptability with respect to gradation of total aggregate for surface-course mixtures.

PERCENT OF AGENCIES ACCEPTING BITUMEN CONTENT

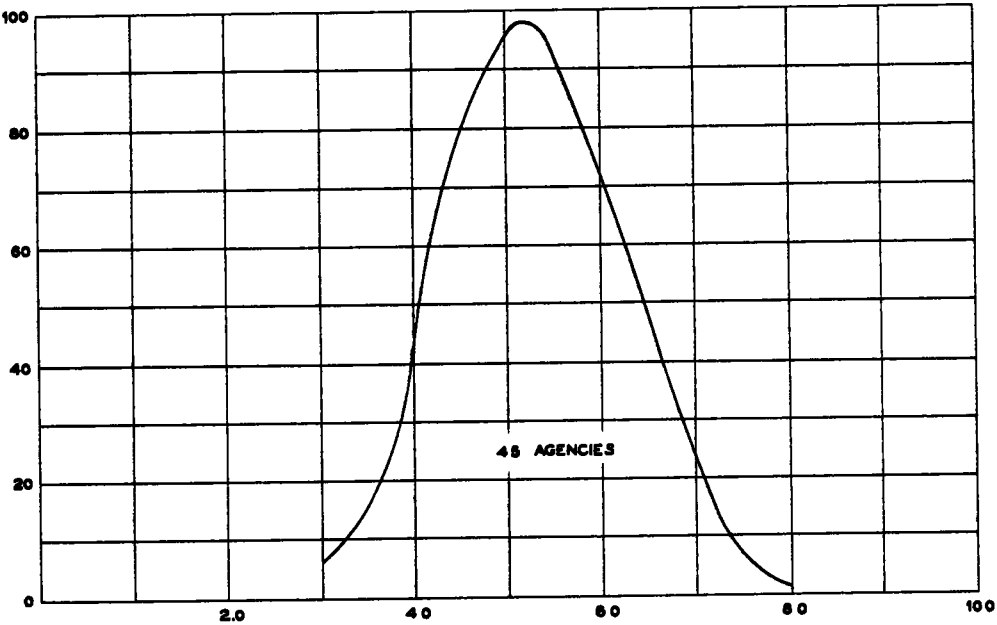

(A) BINDER-COURSE MIXTURES

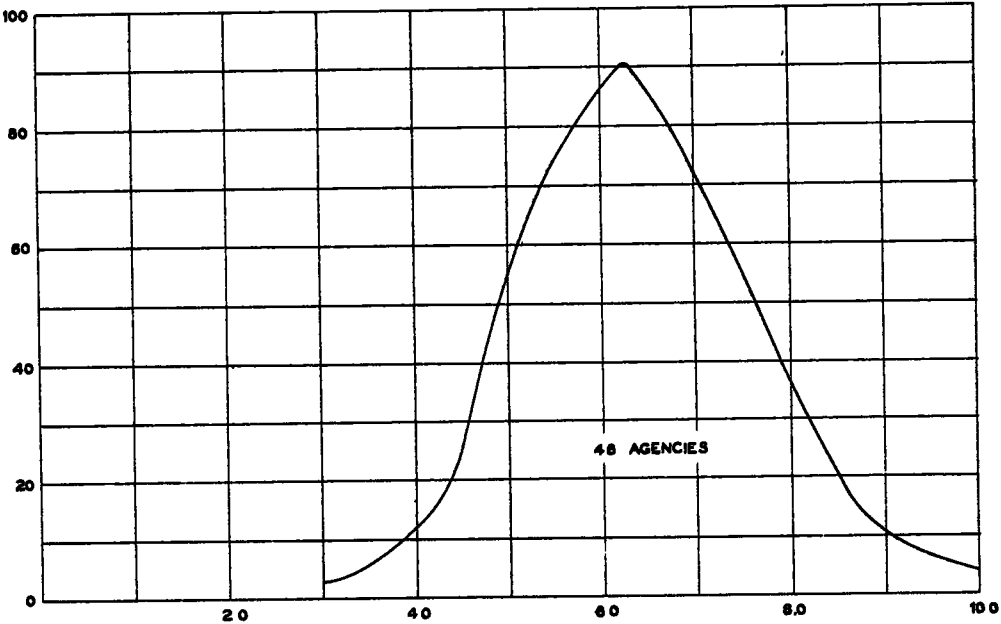

(B) SURFACE-COURSE MIXTURES

BITUMEN CONTENT - PERCENT OF TOTAL MIXTURE

Figure 9. Frequency of acceptance of percents of bitumen in total mixture.

of the points at which the straight lines intersected the vertical lines of the semilogarithmic chart representing the more commonly used sieves. The tabulation of these values for binder-course mixtures is shown in Table 5-b, and for surface-course mixtures in Table 6-b.

**Binder Course.** From the values given in Table 5-b, the frequency of acceptance of the various percentage values passing each of the selected sieves was determined and plotted for all agencies. The frequency-of-acceptance curves for all agencies were then drawn as shown in Figure 5. It will be noted from these frequency-of-acceptance curves that, although the complete range of percentage limits for any one

TABLE 7-8-a  
SPECIFIED TOLERANCES FROM JOB-MIX FORMULAS

Sieve Size or Number	Number of Agencies	Average of 1/ Reported Tolerance Figures % ( $\pm$ )	Number of Agencies Within <sup>†</sup> One Percentage Point of Average	Range of Tolerances Reported % ( $\pm$ )
<u>Binder-Course Mixtures</u>				
3/4"	26	6	18	3-10
1/2"	29	6	21	3-10
3/8"	27	6	13	3-12
No. 4	36	5	23	2-10
No. 10	29	4	23	2-10
No. 20	12	4	12	3-5
No. 40	22	4	18	2-10
No. 80	17	3	13	2-5
No. 200	31	2	26	0.5-4
Asphalt	38	0.4	34 <sup>2/</sup>	0.2-1.0
<u>Surface Course Mixtures</u>				
1/2"	27	6	18	2-10
3/8"	34	6	23	2-10
No. 4	37	5	29	2-10
No. 10	36	4	31	2-10
No. 20	26	4	24	2-5
No. 40	32	4	27	2-8
No. 80	29	3	25	2-5
No. 200	41	2	34	0.5-5
Asphalt	39	0.4	33 <sup>2/</sup>	0.2-1.0

1/ Total of 42 agencies reporting

2/ Within  $\pm$  0.1 percentage point of average

sieve is relatively great, there is still a definite tendency toward concentration of acceptance within a relatively narrow range. This is further demonstrated in Figure 6 where are shown various concentrations of agencies with respect to acceptance of percentages of mineral aggregate passing the entire range of sieves. The method of developing these envelopes is the same as that previously described for the development of the envelopes for fine aggregate.

It is generally accepted that, for optimum performance, the grading of a mineral aggregate from coarse to fine must vary somewhat in relation to the maximum size of aggregate. The practices of the agencies grouped according to top-size of aggregate for the more frequently used top sizes were examined in a manner similar to that previously described for the agencies as a whole. For binder-course aggregates, the most frequently used top sizes (based on 90 percent of material passing, as shown in Table 5-b), are the 1-in. and  $\frac{3}{4}$ -in. top sizes. The results of this examination are also shown in Figures 5 and 6. It will be noted from the figures that grouping of the agencies by top sizes of aggregate produced a greater degree of concentration with respect to acceptance of percentages of material passing all sieves.

**Surface Course.** Surface-course-aggregate gradation limits were examined in the same manner as were the binder-course-aggregate limits. The results of the plottings are shown in Figures 7 and 8. It will be seen from these figures that similar results were obtained.

**Asphalt Content.** Forty-six of the 50 reporting agencies indicate that maximum and minimum asphalt contents are specified for binder-course mixtures. All but five of the agencies use the total mixture as a basis for specifying asphalt content. The remaining five specify asphalt content as a percentage of the total aggregate.

For the agencies reporting (converting the limits for the agencies using the total-aggregate basis to a total-mixture basis), the specified percentages range from a low of 2.9 percent to a high of 8.0 percent for binder-course mixtures, and from a low of 2.9 percent to a high of 10 percent for surface-course mixtures. Frequency-distribution curves for acceptance of various asphalt contents are shown in Figure 9(a) for binder course materials, and in Figure 9(b) for surface-course materials. Average values for the lower and upper limits for asphalt content of binder-course mixtures are 4.1 percent and 6.4 percent respectively, and average values for the lower and upper limits for surface-course mixtures are 5.0 percent and 7.5 percent respectively.

### Job-Mix Formula

In addition to the controls previously discussed, most agencies require that a single combination of aggregate and asphaltic material, known as the "Job-Mix Formula," be determined for each project. The job-mix formula must of course be within the limits of the specifications. Small tolerances from the job-mix formula are specified. The job-mix formula is usually determined from trial mixes or from previous experience with the aggregates at hand.

Forty-two agencies indicate the use of job-mix formulas and specified tolerances therefrom for binder-course mixtures, and the same number also for surface-course mixtures. Summary information concerning tolerances for the more commonly used sieves, and for asphalt content is presented in Table 7-8-a. It will be noted that practice is reasonably consistent.

TABLE 9-a  
USAGE OF STABILITY TESTS IN DESIGNING  
BITUMINOUS-CONCRETE MIXTURES

Stability Test	Number of Agencies	Tests Used in Addition to Those Listed in First Column	Number of Agencies
Marshall	20	Ruohard-Field Hveem Triaxial Compression	3 1 1
Hveem	12	Marshall	1
Ruohard-Field	11	Marshall Immersion-Compression	3 1
Unconfined Compression	2	Immersion-Compression and Vibrating Table	1
Triaxial Compression	2	Marshall	1
Immersion-Compression	2	Ruohard-Field Unconfined Compression and Vibrating Table	1 1
Vibrating Table	2	Unconfined Compression and Immersion-Compression	1
Direct Compression	1		
Practical experience - no specific test	5		
Total of 45 agencies reporting			



## MIXTURE DESIGN

### Stability Tests

Most of the reporting agencies use at least one of the special tests that are available as guides in designing for stability in bituminous-concrete mixtures. Of 49 agencies reporting, only five indicate that no method other than trial and error is used in at least the preliminary determination of proper mixture composition with respect to stability. The usage of the various stability tests is summarized in Table 9-a. It will be noted that the most popular stability tests are the Marshall (20 agencies), the Hveem (12 agencies), and the Hubbard-Field (11 agencies).

### Stability Test Figures

The ranges in test figures that are considered by the reporting agencies to be indicative of satisfactory mixtures are shown in Table 9-b for the tests receiving major usage. The ranges are listed without regard to the characteristics of the aggregates and bituminous materials contained in the mixtures to which they have been applied. They must therefore not be considered to have universal application.

### Specifications Based on Stability Tests

Eleven of the reporting agencies state that they include in their specifications requirements that are based on stability tests. Nine of these state that their specified values are based on standard tests and test procedures. The limiting figures specified by these nine agencies are tabulated in Table 9-c. It will be seen from the table that these particular specifications are far from standardized, with no two agencies specifying identical groups of limiting figures.

### Specific Gravity in Mixture Design

Experience has shown that bituminous-concrete mixtures perform best at a relatively narrow range of densities below a given voidless maximum. The maximum density to which compacted mixtures are usually referenced is a theoretical voidless density calculated through the use of specific gravity figures for the individual constituents of the mixture.

If aggregate absorbed no asphalt, or if the voids within the aggregate particles became completely filled with asphalt, the choice of specific-gravity figures for use in theoretical calculations would be a simple matter. However, it is most common for the voids in the aggregate particles to become partially filled with asphalt. Therefore, the specific-gravity figures that are used for the aggregates are frequently a compromise, although some effort has been directed toward the determination of specific-gravities that more accurately represent actual conditions. Usage among the reporting agencies with regard to specific gravities assumed for aggregates in theoretical-density calculations is shown on the following page.

TABLE 9-b  
LIMITING STABILITY TEST FIGURES USED IN THE DESIGN AND CONTROL  
OF BITUMINOUS CONCRETE MIXTURES  
(For Tests Receiving Major Usage)

Test	Traffic Unif	Number of Agencies	For Medium Traffic	Number of Agencies	For Heavy Traffic	Number of Agencies
<b>Marshall Method 1/</b>						
Stability, lbs	500+	1	500+	1	1500+	5
	1000+	2	600+	1	2000+	1
	1000 to 1500	1	1000+	3		
	1500+	1	1200+	1		
Flow, 0.01 in	12	1	12-20	1	8-18	1
	15	1				
	15-	3				
	20-	4				
	8-18	1				
	10-15	1				
	12-18	1				
Density, pct of theoretical 2/3/	90 B	1				
	92-96 B	1				
	96 B	1				
	94-96 B	1				
	94-98 B	1				
	95-97 B	3				
	93-97 A	1				
	94-98 A	1				
	94-97 E	1				
	94-98 E	1				
Voids Filled with Asphalt, percent 2/	65-85 E	1				
	75-85 E	1				
	75-85 B	2				
	93-97 A	1				
<b>Hveem Stabilometer Method 1/</b>						
Stabilometer Value, pct	30+	1				
	35+	4				
	40+	1				
	35-50	2				
Cohesimeter Value	50+	1				
	94-98	1				
	92+B	1				
	94-98 A,B	1				
<b>Hubbard-Field Method 1/</b>						
Stability, lbs	1500	1	1200	1	2000	1
	3000+	1	1500	1	2500	1
			3000 to 4500	1	3000	1
Density, pct of theoretical 2/3/	94-97 A,B	1				
	95-98 S	1				
	90 B	1				

1/ Figures are not included for agencies indicating modified testing methods  
2/ Specific gravities used in determining theoretical densities and void contents  
B = Bulk V = "Vacuum saturated"  
A = Apparent S = Bulk, surface dry basis  
E = "Effective"

3/ For agencies reporting voids limitations rather than density limitations, the complementary density limitations have been tabulated to facilitate comparison

<u>Specific Gravity</u>	<u>Number of Agencies</u>
Bulk (ASTM)	19
Apparent (ASTM)	14
Bulk and Apparent	5
Bulk, Surface Dry Basis (ASTM)	3
"Effective"	2
"Vacuum Saturated"	1

**CONSTRUCTION REQUIREMENTS**

As mentioned previously, the questionnaires were for the most part designed to obtain information on items where some choice was likely to be involved insofar as the preparation of the construction specifications for the AASHTO Test Road was concerned. Questions were usually not asked about detailed specification re-

quirements and practices which were recognized as intrinsic in the control of bituminous-concrete construction and as being common to all agencies practicing bituminous-concrete construction. The absence of information on these details occurs perhaps with greatest frequency in the portions of the report dealing with construction and equipment requirements. This should be borne in mind by anyone making use of the information which is herein presented.

TABLE 9-c

LIMITING STABILITY TEST FIGURES USED IN  
BITUMINOUS-CONCRETE SPECIFICATIONS  
(For Agencies Using Standard Test Procedures)

Stability Test	Stability Figures	<u>Specified Limiting Test Figures</u>	
		Flow (0.01 in.)	Density $\frac{1}{2}$ / (pct. theoretical)
Marshall (La.) (S.C.)	1000+ 600+ med. traffic; 2000+ heavy "	8-18	92-96 B
Hveem (Okla.) (Cal.) (Me.)	35+ 35+ 35-50		94-98 A,B
Hubbard-Field (Mo.) (Mont.) (Fla.)	3000+ - 1200 med. traffic; 3000 heavy "		94-97 A,B 95-98 S
(Va.)	1500 med. traffic; 2000 heavy "		95-98 (Asphalt Institute)B 90 B

1/ For agencies reporting voids limitations rather than density limitations, the complementary density limitations have been tabulated to facilitate comparison.

2/ Specific gravities used in determining theoretical density:

A = Apparent

B = Bulk

S = Bulk, surface dry basis

## PREPARATION OF MATERIALS

### Mineral Aggregates

**Storage.** Forty-four of the reporting agencies state that their specifications require that when different sizes of aggregate are furnished separately for bituminous-concrete mixtures, each size that is furnished is to be maintained in a separate stockpile. The six remaining agencies have no such requirement, presumably because aggregates are not furnished in separate size fractions.

Twenty-seven agencies report specification statements requiring a general absence of segregation, degradation and intermixing of materials. Eleven agencies report having no such statement, and 12 agencies did not report.

Only 13 agencies report having specification requirements covering the construction of stockpiles. Four require that stockpiles be constructed in lifts 3 ft or less in thickness, 4 others require that lifts be 4 ft or less in thickness, one requires that the lifts be 5 ft or less, and 4 require only that the stockpiles be constructed in lifts.

**Heating and Drying.** Forty-six agencies reported on temperatures specified for the heating of the aggregate. One agency reports only that its requirements vary with conditions, one agency reports having no specification requirement, and two agencies did not report. Thirty-two specify temperature ranges, and 14 specify maximum limitations only. Reference to Part a of Table 10-a will show that there is considerable variation in the temperature ranges or maximum limiting temperatures that are specified for aggregate. Twenty-five different ranges or maximum limitations are reported. The greatest number of agencies specifying any one range is five; these specifying a range of 250 F to 325 F. The greatest number of agencies specifying the same maximum limitation is nine; these specifying a limitation of 325 F.

Considering specified maximum and minimum limitations rather than ranges, practice appears more consistent. As will be seen from Part b of Table 10-a, only four different minimum limits are specified. A minimum of 250 F, specified by 15 agencies, is used most frequently. There will be seen to be a somewhat greater diversity of practice in maximum limits specified, although 17 agencies specify a 325 F maximum and 10 specify a 350 F maximum.

Three agencies have differing temperature requirements for binder-course and surface-course mixtures, as will be seen from Table 10-a.

**Moisture Retention.** Only 15 agencies report specifying a maximum percentage limitation on the amount of moisture allowed to be contained in mineral aggregate at

TABLE 10-a  
SPECIFIED TEMPERATURES FOR HEATING  
AND DRYING MINERAL AGGREGATES

a. Agencies grouped according to specified temperature range			
Specified Temperature Range of.	Number of Agencies	Specified Temperature Range of.	Number of Agencies
225-275	1	300-350	1
225-300	1	300-375	2
225-325	2	300-385	1
225-350	2(1-B) <sup>1/</sup>	300-400	1
250-300	1	300 max.	1
250-320	1	325 max.	9
250-325	5	350 max.	2
250-340	1	375 max.	1
250-340	3(1-B)	400 max.	(1-B)
250-375	2	425 max.	(1-B)
250-400	1	Varies	1
275-325	1	Not specified	1
275-335	1	Not reported	2
275-350	2		
275-375	(2-B)	Total agencies	50

b. Agencies grouped according to specified upper temperature limit and according to specified lower temperature limit			
Specified Lower Limit of.	Number of Agencies	Specified Upper Limit of.	Number of Agencies
225	6(1-B) <sup>1/</sup>	300	3
250	15(1-B)	325	17
275	4(2-B)	350	10(2-B)
300	5	375	5(2-B)
		400	3(1-B)
		Other	5(1-B)

<sup>1/</sup> Three additional agencies report specifying different temperature ranges for binder-course and surface-course aggregates. The numerals within parentheses indicate the number of agencies, the letter "B" indicates binder-course aggregate, the letter "S" indicates surface-course aggregate.

TABLE 10-b  
SPECIFIED LIMITATIONS ON AMOUNT OF MOISTURE TO BE  
CONTAINED IN MINERAL AGGREGATE AT TIME OF MIXING

Specified Maximum Moisture Content	Number of Agencies
Percent of dry weight	
0.0	1
0.2	1
0.5	2
1.0	9
1.25	1
2.0	1
"Dry"	8
"Trace"	1
"No foaming"	3
Not specified	20
Not reported	3
Total agencies	50

the time of mixing. As will be seen from Table 10-b, percentage limitations that were reported vary from 0.0 percent to 2.0 percent, with 9 agencies specifying a maximum moisture content of 1.0 percent. Eight agencies report that they require the aggregate to be "dry," one permits a "trace" of moisture, and three require that the moisture content be such that there will be "no foaming." Twenty agencies report having no specification requirement covering moisture retention.

### Asphalt Cement

Eighteen different temperature specifications for heating asphalt cement were reported by forty-three agencies. Thirty-seven of these agencies specify a range of temperature to within which the asphalt must be heated, five specify a maximum limitation only, and one specifies a minimum limitation only. Practice concerning the specified limitations is summarized in Table 10-c. It will be seen from Part a of Table 10-c that the greatest number of agencies specifying any single range is the ten that specify a range of 250 F to 350 F. No more than seven specify any other range, or single maximum or minimum limitation.

From Part b of Table 10-c it will be seen that when maximum and minimum limitations are considered rather than ranges, only five different figures were reported for each. Of these, a 250 F limitation is specified as a minimum most frequently (21 agencies), and 350 F limitation is specified as a maximum most frequently (15 agencies).

## PREPARATION OF MIXTURES

### Batch-Type Mixing Plants

#### Mixing Period

Data regarding required mixing periods for batch-type mixers are summarized in Table 10-d.

Twenty-six agencies report that a minimum number of seconds of dry mixing are required. The specified minimums range from 5 to 20 seconds, with 19 agencies specifying a 15-second minimum dry-mix period. One additional agency specifies a minimum dry-mix period of 15 seconds for surface-course mixtures and 5 seconds for binder-course mixtures. Twelve agencies require only that mixing of the dry material shall be "thorough."

Forty-seven agencies reported on specified minimum wet-mix periods. Specified minimums range from 20 to 55 seconds. Twenty-one agencies specify a minimum of 30 seconds, and 19 specify a minimum of 45 seconds. One other agency specifies a minimum wet-mix period of 45 seconds for surface-course mixtures and a minimum of 35 seconds for binder-course mixtures.

Forty-one agencies report that a minimum total-mix period is specified in seconds. The minimum periods that are specified range from 30 seconds to 90 seconds. Thirteen specify a minimum total-mix period of 45 seconds, and 10 specify a minimum period of 60 seconds. One additional agency specifies a minimum total-mix period of 60 seconds for surface-course mixtures and 45 seconds for binder-course mixtures. Another agency specifies 45 seconds for surface-course mixtures and 35 seconds for binder-course mixtures.

TABLE 10-c

#### SPECIFIED TEMPERATURES FOR HEATING ASPHALT CEMENT

a. Agencies grouped according to specified temperature range			
Specified Temperature Range	Number of Agencies	Specified Temperature Range	Number of Agencies
180-350	1	250-300	2
200-300	1	250-325	7
200-325	1	250-340	1
200-400	1	250-350	10
225-275	1	250-400	1
225-300	3	255-295	1
225-325	2	275 min.	1
		275 max	1
		275-325	1
		275-350	4
		300 max	4
		Varies	1
		Not specified	2
		Not reported	4
		Total agencies	50

b. Agencies grouped according to specified upper temperature limit and according to specified lower temperature limit.			
Specified Lower Limit	Number of Agencies	Specified Upper Limit	Number of Agencies
180	1	275	2
200	3	300	10
225	6	325	11
250	21	350	15
275	6	400	2

### Continuous-Type Mixing Plants

#### Mixing Period

Specified minimum mixing periods for

TABLE 10-d  
SPECIFIED MINIMUM MIXING PERIODS FOR MIXTURES  
PREPARED IN BATCH-TYPE MIXING PLANTS

Dry Mix		Wet Mix		Total Mix	
Specified Minimum Mixing Period seconds	Number of Agencies	Specified Minimum Mixing Period seconds	Number of Agencies	Specified Minimum Mixing Period seconds	Number of Agencies
5	2(1-B) <sup>1/</sup>	20	1	30	3
10	3	25	2	35	4(1-B) <sup>1/</sup>
15	19(1-S)	30	21	40	5
20	1	35	(2-B) <sup>1/</sup>	42	1
		40	1	45	13(1-B, 1-S)
"Thorough"	12	45	19(1-S)	50	1
Not specified	4	50	(1-S)	60	10(1-S)
Not reported	8	55	1	70	1
Total agencies	50	Not reported	3	90	1
		Total agencies	50	"Thorough"	1
				Not specified	3
				Not reported	5
				Total agencies	50

<sup>1/</sup> Two agencies report specifying different mixing periods for binder-course and surface-course mixtures. The numerals within parentheses indicate the number of agencies; the letter "B" indicates binder-course mixture; the letter "S" indicates surface-course mixture.

continuous mixing were reported by only 22 agencies. Since the mixing period in continuous mixing cannot be determined directly, these agencies use the following formula to determine the mixing period:

$$\text{Mixing period (sec)} = \frac{\text{Pugmill dead capacity (lb)}}{\text{Pugmill output (lb/sec)}}$$

Reported specified minimum periods vary from 30 seconds to 60 seconds. As will be seen from Table 10-e, there is no great concentration of agencies specifying any single minimum mixing period. Six agencies specify a minimum period of 45 seconds as determined by formula, 5 agencies specify a minimum period of 35 seconds, and an additional agency specifies a minimum period of 45 seconds for surface-course mixtures and 35 seconds for binder-course mixtures.

Twenty-one agencies did not report concerning specifications for a minimum mixing period for continuous mixing, four agencies reported that no minimum period is

TABLE 10-e

SPECIFIED MINIMUM MIXING PERIODS FOR MIXTURES  
PREPARED IN CONTINUOUS-TYPE MIXING PLANTS

Specified Minimum Mixing Period <sup>1/</sup>	Number of Agencies
seconds	
30	4
35	5(1-B) <sup>2/</sup>
40	2
45	6(1-S)
50	2
60	2
Not reported	21
Not specified	3
Type not permitted	4

<sup>1/</sup> Calculated by formula      Seconds =  $\frac{\text{Pugmill Dead Capacity (lb.)}}{\text{Pugmill Output (lb./sec.)}}$

<sup>2/</sup> One additional agency reports specifying different mixing periods for binder-course and surface-course mixtures. The letter "B" indicates binder-course mixture, the letter "S" indicates surface-course mixture.

specified produces less variation. As will be seen from Part b of Table 10-f, four minimum temperatures are principally specified. Among these, a 250 F minimum is specified by 16 agencies (one agency for gravel aggregate only), and a 225 F minimum by 9 agencies. Also from Part b of the table, it will be seen that 5 maximum temperatures are principally specified. Fourteen agencies specify a maximum temperature of 325 F, one of which specifies this temperature only when stone is used. One additional agency specifies this maximum temperature for binder-course material only, and specifies a maximum of 350 F for surface-course material. Eleven other agencies specify a maximum temperature of 350 F.

## PLACING MIXTURES

## Air Temperature

Forty-six of the agencies reported on air temperatures that are specified as minimums for the placing of bituminous-concrete mixtures. Three agencies reported that they do not specify a minimum air temperature at which mixtures are to be placed, and one agency made no report.

As will be seen from Table 10-g, minimum temperatures specified for placing vary from 32 F to 60 F. The single agency specifying the 32 F minimum qualifies this by stating that the temperature must be rising. If the temperature is falling, this agency specifies a minimum of 38 F. Only one other agency specifies one minimum for use when the temperature is rising and another for use when the temperature is falling. A total of 28 agencies specify a minimum air temperature of 40 F, and another specifies 40 F when the temperature is falling. Six agencies specify 35 F as a minimum, and one specifies 35 F when the temperature is rising. Six others specify a minimum

specified, and four agencies do not permit the use of a continuous-type mixer.

## Both Types of Mixing Plant

## Mixture Temperature at Discharge

All but 4 of the 50 reporting agencies have specifications covering temperatures for material at discharge from the mixer. Thirty-seven of these specify minimum and maximum temperatures between which the temperature of the material must range. Nine specify only a maximum temperature which is not to be exceeded. As will be seen from Part a of Table 10-f, practice is quite varied as to specified ranges. The only single range that is specified by more than 3 agencies is the 250 F - 350 F range that is specified by 6 agencies. Grouping of agencies by minimum and maximum temperatures

TABLE 10-f

## SPECIFIED TEMPERATURES FOR MIXTURE AT DISCHARGE FROM MIXER

a Agencies grouped according to specified temperature range <sup>1/</sup>			
Specified Temperature Range °F.	Number of Agencies	Specified Temperature Range °F.	Number of Agencies
200-300	1(1-gravel) <sup>2/</sup>	265-325	1
200-350	1	275-325	2
225 min	1	275-350	2
225-275	2	280-375	1
225-300	2	300-350	1
225-325	3	300 max	1
225-350	1	310 max	1
235-275	1	325 max	5(1-B) <sup>2/</sup>
250-275	1	350 max	1(1-S)
250-280	1	375 max	1
250-300	3	Not specified	4
250-325	3(1-stone) <sup>2/</sup>		
250-340	1		
250-350	6		
275-325	1		
260-375	1		

b Agencies grouped according to specified upper temperature limit and according to specified lower temperature limit <sup>1/</sup>			
Specified Lower Limit °F.	Number of Agencies	Specified Upper Limit °F.	Number of Agencies
200	2(1-gravel) <sup>2/</sup>	275	4
225	9	300	7(1-gravel) <sup>2/</sup>
250	15(1-stone) <sup>2/</sup>	325	14(1-B) <sup>2/</sup> (1-stone) <sup>2/</sup>
275	4	350	11(1-S)
Other	6	375	3
		Other	4

<sup>1/</sup> One additional agency reports specifying one temperature range for mixtures containing stone, and another for mixtures containing gravel. The materials within parentheses indicate the number of agencies.

<sup>2/</sup> One additional agency reports specifying different temperature ranges for binder-course and surface-course mixtures. The material within parentheses indicates the number of agencies, the letter "B" indicates binder-course mixture, the letter "S" indicates surface-course mixture.

air temperature of 50 F for placing.

### Mixture Temperature at Placing

Forty-three agencies reported on specifications for mixture temperature at the time of placing. Thirty-six of these specify maximum and minimum temperatures within which the temperature of the mixture must range. Included are three agencies that specify differing limits for binder-course and surface-course material, and one agency that specifies one set of limits for gravel aggregate and another set for stone aggregate. Three agencies specify only minimum limits, and three others specify only maximum limits. Five agencies report no specification, and two agencies did not report.

As was true for the specifications concerning mixture temperatures at discharge, few agencies specify any single specific range (see Table 10-h, Part a). The greatest number of agencies specifying any single range is the four that specify the 225 F to 325 F range. Two additional agencies specify this range for binder-course mixtures only.

As was also true for specified temperatures at discharge, grouping of agencies by specified minimum and maximum temperatures produced less variation. As will be seen from Part b of Table 10-h, four minimum temperatures and five maximum temperatures are principally specified. A 225 F minimum is specified by 14 agencies and a 250 F minimum by 12 agencies. In addition, two agencies specify the 225 F minimum for binder-course mixtures, and one specifies this minimum for use only with stone aggregate. Also, one agency specifies the 250 F minimum for binder-course mixtures only, and three specify the minimum for surface-course mixtures only. Twelve agencies specify a 325 F maximum and nine specify a 300 F maximum. Three additional agencies specify the 325 F maximum for binder-course mixtures alone, and one additional agency specifies the 300 F maximum when crushed-stone aggregate is used.

### Daily Tolerance in Temperature

Specifications controlling the maximum daily variations in mixture temperature were reported by 33 agencies. Thirteen agencies report having no such specification, and four agencies did not report. The information on tolerances is summarized in Table 10-i. It will be seen from the table that specified tolerances ranged from  $\pm 10$  F to  $\pm 30$  F. Seventeen of the agencies specify a tolerance of  $\pm 20$  F, and 8 agencies specify a tolerance of  $\pm 25$  F.

### Spreading and Finishing Machine Speed

Operating speeds for spreading and finishing machines are reported to be specified by 20 of the reporting agencies. Eleven report having no specification regarding speed, and the remaining 9 either did not report, or reported a general statement which has the effect of indirectly controlling speed. Some, or all, of those reporting that a speed is not specified probably also have some form of indirect control.

Twelve of the 20 agencies with speed regulations specify a speed range within which the machine must operate. Eight specify a maximum speed which is not to be exceeded. One of these 8 specifies one maximum speed for binder-course mixtures and another for surface-course mixtures. As will be seen from Table 10-j, no single range, or maximum value when only a maximum speed is specified, is specified by a large

TABLE 10-g  
SPECIFIED MINIMUM AIR TEMPERATURES AT  
WHICH MIXTURES MAY BE PLACED

Specified Minimum Air Temperature °F.	Number of Agencies
32	(1-rising) <sup>1/</sup>
35	6(1-rising)
36	1
38	(1-falling)
40	2(1-falling)
45	2
50	6
60	1
Not specified	3
Not reported	1
Total agencies	50

<sup>1/</sup> Two additional agencies report specifying two minimum air temperatures for placing mixtures, one minimum temperature when the temperature is rising and another when the temperature is falling. The numeral within parentheses indicates the number of agencies.

TABLE 10-h

## SPECIFIED TEMPERATURES FOR MIXTURE AT PLACING

a. Agencies grouped according to specified temperature range			
Specified Temperature Range °F	Number of Agencies	Specified Temperature Range °F	Number of Agencies
175-275	(1-gravel) <sup>1/</sup>	250-350	2(3-S)
200-300	2	250-375	1
200-350	1	255-305	1
225 min.	1	265-325	1
225-255	1	275 max.	1
225-275	2	275-325	3
225-300	3(1-stone)	280-375	1
225-325	4(2-B) <sup>2/</sup>	300 max.	1
225-350	3	325 max.	1
240 min.	1	Not specified	5
250 min.	1	Not reported	2
250-275	1		
250-300	3		
250-325	3(1-B)		
250-340	1		
b. Agencies grouped according to specified upper temperature limit and according to specified lower temperature limit			
Specified Lower Limit °F	Number of Agencies	Specified Upper Limit °F	Number of Agencies
200	3	275	4
225	14(1-stone) <sup>1/</sup> (2-B) <sup>2/</sup>	300	9(1-stone)
250	12(1-B)(3-S)	325	12(3-B)
275	3	350	6(3-S)
Other	4	375	2
		Other	3

<sup>1/</sup> One agency reports specifying different temperature ranges for stone and gravel in the bituminous mixture. The numerals within parentheses indicate the number of agencies; "stone" and "gravel" indicates the aggregate used.

<sup>2/</sup> Three agencies report specifying different placing temperature ranges for binder-course and surface-course mixtures. The numeral within parentheses indicates the number of agencies; the letter "B" indicates binder-course mixtures; the letter "S" indicates surface-course mixtures.

group of agencies. The greatest number specifying any single range is the four that specify that the operating speed of the spreading and finishing machine be between 10 and 30 ft per min. Of the agencies specifying maximum speed only, the greatest number specifying a single value is the three that specify a maximum of 30 ft per min. One additional agency that specifies one maximum speed for surface-course mixtures and another for binder-course mixtures specifies a maximum of 30 ft per min for binder-course mixtures.

#### Lift Thickness

Information concerning lift thicknesses that are specified and lift thicknesses that are normally placed was obtained from the questionnaires and is summarized in Table 10-k. Thirty agencies report that a maximum lift thickness is specified for the binder course, and 35 agencies report that a maximum thickness is specified for the surface



TABLE 10-1  
SPECIFIED MAXIMUM DAILY TOLERANCES FROM  
ESTABLISHED TEMPERATURE FOR MIXTURE AT PLACING

Specified Daily Temperature Tolerance ° F.	Number of Agencies
10	2
15	3
20	17
25	8
30	3
Not specified	13
Not reported	4
Total agencies	50

and 2-in. courses (6), than any other thicknesses. Normally-placed thicknesses of surface course range between 1 in. and 2½ in., with more agencies placing 1½-in. courses (14), and 1-in. courses (8), than any other thicknesses.

### Rolling Requirements

**Type and Number of Rollers.** Data regarding the type and number of rollers that are required are summarized in Table 10-1 and Table 10-m. In Table 10-1 are summarized requirements for roller type. Tandem, three-wheel, and pneumatic rollers are all used to some extent. Of 49 agencies reporting that they specify the type of roller to be used, 16 specify that either tandem or three-wheel rollers may be used, another 16 specify that a minimum of one tandem roller and one three-wheel roller is to be used, and 11 specify that tandem rollers alone may be used. Other combinations of the three types of rollers are used much less extensively. Only six agencies permit a pneumatic roller to be used.

From Table 10-m it will be seen that two agencies specify that a minimum of three rollers are to be used (for each spreading and finishing machine), and 25 agencies specify that a minimum of two rollers are to be used. The remaining 23 reporting agencies apparently do not specify a minimum number of rollers to be used. It will be further noted that the most frequently required combination is a minimum of one tandem roller and one three-wheel roller (by 14 agencies).

**Tonnage and Roller Speed.** Thirty-two agencies set a specific maximum amount of material that may be placed per hour for each roller that is used. Twenty-seven of these state the amount of material on a ton-per-roller-hour basis, and five use a square-yard-per-roller-hour basis. Maximum-tonnage values, as will be seen from Table 10-n, range from 25 tons per roller-hour to 150 tons per roller-hour. The most frequently specified maximum tonnages per roller-hour that are specified are 40 (6 agencies), 30 (5 agencies) and 50 (4 agencies).

course. One agency controls thickness by specifying a maximum lb per sq yd of material that may be placed. Specified maximum thicknesses for binder courses range between 1 in. and 3 in. Twelve agencies specify 2 in., 8 agencies specify 3 in., and 6 agencies specify 1½ in. Specified maximum thicknesses for surface courses range between 1 in. and 3½ in. Fourteen agencies specify 2 in., 9 agencies specify 1½ in. and 4 agencies specify 1 in.

Lift thickness of binder courses normally placed was reported by 34 agencies, and for surface courses by 39 agencies. Normally-placed thicknesses of binder course range between 1 in. and 3 in., with more agencies placing 1½-in. courses (15),

TABLE 10-j  
SPECIFIED OPERATING SPEEDS FOR  
SPREADING AND FINISHING MACHINE

Specified Operating Speed ft. per min	Number of Agencies
5-20	1
5-30	1
5-50	1
7-26	1
10-20	4
10-30	2
10-50	1
20 max.	2(1-8) <sup>1/</sup>
20-25	1
25 max.	1
30 max.	3(1-3)
35 max.	1
As required	1
Avoid tearing	2
Not specified	11
Not reported	16
Total agencies	50

<sup>1/</sup> One additional agency reports specifying different maximum speeds for binder-course and surface-course mixtures. The numeral within parentheses indicates the number of agencies; the letter "B" indicates binder-course mixture, the letter "S" indicates surface-course mixture.

TABLE 10-k  
LIFT THICKNESSES - MAXIMUM SPECIFIED  
AND THICKNESS NORMALLY USED

Specified Maximum Thickness				Thickness Normally Placed			
Binder Course inches	Number of Agencies	Surface Course inches	Number of Agencies	Binder Course inches	Number of Agencies	Surface Course inches	Number of Agencies
1	1	1	4	1	1	1	8
1 1/4	1	1 1/4	1	1-1 1/2	1	1-1 1/2	2
1 1/2	6	1 1/2	9	1-2	1	1-2	2
2	12	2	14	1-3	1	1 1/4	5
2 1/2	2	2 1/2	4	1 1/4	2	1 1/2	14
3	8	3	2	1 1/2	15	1 1/2-2	2
170 lbs. <sup>1/</sup>	1	3 1/2	1	1 1/2-2	1	1 1/2-2 1/2	1
Var.	1	130 lbs. <sup>1/</sup>	1	1 1/2-2 1/2	1	2	3
N.R. <sup>2/</sup>	17	Var.	1	1 3/4	1	2 1/2	2
Not used	1	N.R.	13	2	6	100 lbs. <sup>1/</sup>	1
Total agencies	50	Total	50	2-3	3	N.R.	10
				2 1/2	1	Total	50
				Not used	1		
				N.R.	15		
				Total	50		

<sup>1/</sup> Lbs. per sq. yd.

<sup>2/</sup> Not reported.

Only 24 agencies report specifying a maximum roller speed. Seven agencies report a requirement to the effect that the speed is to be such that displacement under the roller will be avoided. It is possible that some of the agencies reporting no requirement may have a requirement similar to that which was reported by these seven agencies. Reported maximum allowable speeds (see Table 10-o) range from 1.5 mph to 3 mph, with most agencies (15) specifying 3 mph.

#### Compacted Density

The questions that were asked con-

TABLE 10-1  
TYPES OF ROLLERS REQUIRED

Roller Type	Number of Agencies
Tandem or three-wheel	16
Tandem and three-wheel, minimum	16
Tandem only	11
Tandem, three-wheel, or pneumatic	2
Tandem or pneumatic	1
Tandem, three-wheel, and pneumatic	3
Not specified	1
Total agencies	50

TABLE 10-m  
MINIMUM NUMBER OF ROLLERS REQUIRED

Minimum Requirement	Number of Agencies
Three rollers	
(a) Two tandem or three-wheel and one pneumatic	1
(b) One 3-axle tandem, others tandem, three-wheel or pneumatic	<u>1</u>
Total agencies	2
Two rollers	
(a) One tandem and one three-wheel	14
(b) Tandem or three-wheel	5
(c) Tandem only	4
(d) Two tandem, or one tandem and one three-wheel	<u>2</u>
Total agencies	25
Minimum not specified	
(a) Tandem or three-wheel	9
(b) Tandem only	8
(c) Tandem, three-wheel or pneumatic	1
(d) Tandem, three-wheel and pneumatic	1
(e) Tandem and three-wheel	2
(f) Tandem or pneumatic	1
(g) Type not specified	<u>1</u>
Total agencies	23

TABLE 10-n  
MAXIMUM TONNAGE SPECIFIED PER ROLLER-HOUR

Specified Maximum Tonnage Per Roller-Hour	Number of Agencies
25	3
30	5
35	2
37½	1
40	6
50	4
75	2
80	1
100	2
150	1
54 yd requirement <sup>1/</sup>	6
Not specified	5
Not reported	12
Total agencies	50

<sup>1/</sup> Six agencies have a requirement based on square yards placed per hour rather than on tonnage. These requirements vary from 200 to 500 sq. yds maximum placement per roller-hour.

cerning density specifications and criteria were unfortunately not sufficiently specific to indicate the amount of information that was needed to completely compare and analyze practice with regard to layer density. Many of the replies that were received were therefore not sufficiently complete to permit a detailed examination of them. Such summarization as was possible is presented in Table 10-p. It will be noted from the table that, while the general range of density that is sought is, with a few exceptions, relatively narrow, the actual limiting figures that are listed are quite varied. Several different bases are also used in arriving at standard densities to which the compacted-layer densities are compared.

For binder courses, 21 agencies report that they specify relative-density requirements. An additional 8 agencies report relative densities that they attempt to meet, but which they do not specify. Of this total of 29 agencies, 11 relate the compacted density to a voidless density calculated through the use of the apparent specific gravity (ASTM) of the aggregates, 6 relate the compacted density to a voidless density calculated through the use of the bulk specific gravity (ASTM) of the aggregates, one uses density obtained by the Hubbard-Field laboratory procedure as a standard, and 3 use a density obtained by the Marshall procedure as a standard. Among the remaining 8 are 2 that report using other specific gravities of aggregates in determining voidless density (surface dry and vacuum saturated), and 6 that did not report in such a way that their standard could be classified.

For surface courses, 25 agencies report specifying relative-density requirements. Eight others report having relative densities that they attempt to meet but do not specify. Of this total of 33 agencies, 13 relate compacted density to voidless density based on the apparent specific gravity of the aggregates, 7 relate compacted density to void-

TABLE 10-o  
SPECIFIED ROLLER SPEEDS

Specified Maximum Speed	Number of Agencies
1.5 mph	2
1.7 mph	1
1.8 mph	1
2 mph	1
2.5 mph	1
3 mph	15
Avoid displacement	7
Not specified	19
Not reported	3
Total agencies	50

less density based on the bulk specific gravity of the aggregates, 2 use a Hubbard-Field density as standard, and 3 use a Marshall density as standard. Two others report calculating voidless densities from other specific gravities of aggregates (surface dry and vacuum saturated), and 6 could not be classified.

TABLE 10-p  
DENSITY REQUIREMENTS FOR COMPACTED LAYERS

Relative Density Requirement			
Binder Course Percent	Number of Agencies	Surface Course Percent	Number of Agencies
<u>Based on Voidless Density Using Apparent Specific Gravity of Materials</u>			
85+	1 (1) $\frac{1}{2}$ $\frac{2}{2}$	85+	(1) $\frac{1}{2}$ $\frac{2}{2}$
90+	1 (1) $\frac{2}{2}$	90+	3 (1) $\frac{2}{2}$
91-96	(1)	91-96	(1)
92+	3	92+	3
94-98	1	92-96	1
95+	1 (1)	94-98	1
97+	(1)	95+	1 (1)
		97+	(1)
<u>Based on Voidless Density Using Bulk Specific Gravity of Materials</u>			
88+	1	90+	1
91-92	(1)	90-95	1
92+	1	91-92	(1)
95+	3	92+	1
		95+	3
<u>Based on Hubbard-Field Laboratory Density</u>			
95+	1	94+	1
		95+	1
<u>Based on Marshall Laboratory Density</u>			
95-99	1	95-99	1
98	1	98	1
Vary with job	1	Vary with job	1
<u>Miscellaneous, or Basis Not Reported</u>			
	8		8
<u>Not Specified</u>			
	14		13
<u>Not Reported</u>			
	7		4

1/ Numbers in parentheses indicate number of additional agencies reporting that they desire, but do not specify, the indicated figures.

2/ One agency desires the 85+ percent for bituminous concrete placed on flexible base, and 90+ percent for bituminous concrete placed on rigid base.

TABLE 10-q  
REQUIREMENTS FOR SURFACE SMOOTHNESS

<u>Binder Course</u>		<u>Surface Course</u>	
Maximum Variation	No. of Agencies	Maximum Variation	No. of Agencies
1/10 in. in 10 ft.	1	1/10 in. in 10 ft.	1
1/8 in. in 16 ft. <sup>1/</sup>	1	1/8 in. in 16 ft. <sup>1/</sup>	2
1/8 in. in 10 ft.	4	1/8 in. in 10 ft.	14
1/16 in. per ft.	1	3/16 in. in 10 ft.	11
3/16 in. in 10 ft.	3	1/4 in. in 20 ft.	1
1/4 in. in 16 ft.	4	1/4 in. in 16 ft.	5
1/4 in. in 12 ft.	1	1/4 in. in 12 ft.	2
1/4 in. in 10 ft.	13	1/4 in. in 10 ft.	11
3/8 in. in 10 ft.	2	Not reported	3
1/2 in. in 20 ft.	1		
1/2 in. in 10 ft.	1		
Not specified	11		
Not reported	7		

<sup>1/</sup> One agency specifies this degree of surface smoothness for bituminous concrete placed on rigid base, but permits up to 1/4-in. variation in 16 ft. for bituminous concrete placed on flexible base.

#### Surface Smoothness

Thirty-two agencies reported on surface-smoothness requirements for binder courses, and 47 reported on surface-smoothness requirements for surface courses. The requirements are summarized in Table 10-q. For binder courses, maximum allowable variations range from 1/10 in. in 10 ft to 1/2 in. in 10 ft. For surface courses, maximum allowable variations range from 1/10 in. in 10 ft. to 1/4 in. in 10 ft. A 1/4-in. maximum permissible variation in 10 ft is reported most frequently for binder courses (13 agencies), followed by 1/8 in. in 10 ft (4 agencies), and 1/4 in. in 16 ft (4 agencies). A maximum-variation requirement of 1/8 in. in 10 ft is reported most frequently for surface courses (14 agencies). Other requirements receiving frequent usage for surface courses are 3/16 in. in 10 ft (11 agencies), 1/4 in. in 10 ft (11 agencies), and 1/4 in. in 16 ft (5 agencies).

#### EQUIPMENT REQUIREMENTS

The questions that were asked concerning equipment requirements were for the most part limited to items where differences in practice were believed to exist. The information that is reported is therefore not a detailed description of equipment used in preparing and placing bituminous-concrete mixtures.

## PREPARATION OF MATERIALS

### Cold-Aggregate Bins

Thirty-five agencies reported on equipment generally used to convey aggregates to the cold bins. Of the agencies using cranes and reporting on the specific type of bucket used, 16 reported using a clamshell bucket and 2 reported using a dragline bucket. Twelve agencies use conveyor belts or elevators. Other pieces of specific equipment mentioned were bulldozers (2 agencies) and trucks (1 agency).

Reported requirements for cold-aggregate bins are outlined in Table 11-a. Fifteen agencies reported on the minimum number of bin compartments specified where more than one compartment is required. Nine of these specify 2 compartments and 6 specify 3 compartments. Eight agencies report specifying a minimum of one compartment for each aggregate size, and it is presumed that the other agencies have a similar requirement though it may not be stated specifically.

Requirements for cold-bin capacity, when included in specifications, are stated in general terms (see Table 11-a). Of 16 agencies reporting a definite requirement, 12 require that the capacity be sufficient to supply the full capacity of the mixer or the operating rate of the plant, 3 require that the bin capacity be not less than 3 times the dead-load capacity of the mixer, and one requires that the bin capacity be in excess of the mixer capacity.

### Aggregate Feeders

Forty-three of the reporting agencies require the use of mechanical feeders for conveying cold aggregate to the driers, and seven do not. However, at least two of those that do not have such a requirement indicate that mechanical feeders are used to some extent. Compartment feeders are normally used by 27 agencies, combination feeders by 10 agencies, individual feeders by 7 agencies, and reciprocating-gate feeders by 2 agencies. Four agencies did not report.

Forty agencies report that their feeders are adjustable for proportional feed, two reported that they are not adjustable, and eight agencies did not report. Thirty-six report that their feeders are adjustable for total feed, one reports the feeder not to be adjustable for total feed, and 13 agencies did not report.

Thirty-six agencies report having a general requirement that the feeder be such that adequate control can be exercised, 7 agencies report having no specific requirement of this nature, and the remaining 7 agencies did not report.

### Aggregate Screens

Twenty-nine agencies reported on scalping-screen openings as related to the maximum size of aggregate. Three agencies report that they do not use scalping screens, and 18 agencies did not report. Summarized information on this item appears in Table 11-b. Screen openings will be seen to vary from aggregate size to  $\frac{1}{2}$  in. larger than aggregate size. Twelve agencies report that the screen

TABLE 11-b  
SCALPING-SCREEN USAGE

Screen Opening Related to Maximum Size of Aggregate	Number of Agencies
1/2-in. larger	2
1/4-in. larger	7
1/8-in. larger	12
1/16 in. larger	1
Same size	2
1/8 - 1/4-in. larger	1
1/16 - 1/4-in. larger	2
1/16 - 1/8-in. larger	2
Not used	3
Not reported	18

TABLE 11-a  
REQUIREMENTS FOR COLD-AGGREGATE BINS

Minimum Number of Compartments	Number of Agencies	Bin Capacity	Number of Agencies
4	5	Supply full capacity of mixer or plant rate	12
3	6	Not less than 3 times dead load of mixer	3
On each aggregate size	8	In excess of mixer capacity	1
Varies	1	Not specified	7
Not specified	10	Not reported	27
Not reported	16		

TABLE 11-c  
 REQUIREMENTS CONCERNING SCREENING EFFICIENCY WHERE OVERSIZE  
 AND UNDERSIZE MATERIALS ARE CONSIDERED SEPARATELY

Small Aggregate						Large Aggregate	
Bin No. 1 <sup>1/</sup>		Bin No. 2		Bin No. 3		Bin No. 4	
Agency	Maximum Oversize <sup>2/</sup> percent	Maximum Undersize <sup>2/</sup> percent	Maximum Oversize percent	Maximum Undersize percent	Maximum Oversize percent	Maximum Undersize percent	Maximum Oversize percent
1	5	20	5	10	5		
2	10	15	5	15	5		
3	5	10	5	20	5		
4	5	5	5	10	5	15	5
5	5	15	10	25	5	25	0
6	10	15	15	15	0		
7	10	10	10	10	10		

<sup>1/</sup> The usual practice of designating as Bin No. 1 the bin containing the smallest size of aggregate exclusive of mineral filler has been followed.

<sup>2/</sup> Oversize and undersize determinations are based on tests with laboratory sieves.

openings are  $\frac{1}{8}$  in. larger than maximum aggregate size, and 7 agencies report that the openings are  $\frac{1}{4}$  in. larger. No other single figures were reported as frequently.

Seventeen agencies have established definite requirements concerning screening systems in an effort to control the size-separations of aggregate in the hot-bin compartments (sometimes called "screening efficiency"). Three different types of requirement are used in attaining this control. These are:

1. Separate limitations on the amounts of material larger than and smaller than the established nominal maximum and minimum sizes that will be permitted in a size-group.
2. A limitation on the combined amounts of material larger than and smaller than the established nominal maximum and minimum sizes that will be permitted in a size-group.
3. A limitation on only the amount of material that is smaller than the established minimum size that will be permitted in a size-group (sometimes referred to as "carry-over").

Table 11-c summarizes the requirements that have been established by the seven agencies using the first type of requirement. As will be seen from the table, the maximum amount of oversize permitted in the various size-groups is either 5 or 10 percent of the total material in the size-group for most agencies, with one agency permitting as high as 15 percent for one size-group and two agencies permitting no oversize material in their coarsest size-groups.

Since the finest size-group contains the finest aggregate permitted under the general gradation specifications (assuming that the gradation specifications are met), there is no reason to place a limitation on undersize material to be contained in this size-group. Undersize limitations for the other size-groups range from 5 to 25 percent of the total material in the size-groups, with most agencies specifying either 10 or 15 percent.

Five agencies used the second-named method; that of limiting the combined amount of oversize and undersize material to be contained in any size-group. Four of these require that at least 85 percent of the material in a size-group must meet the established minimum and maximum sizes for the group, when tested with laboratory sieves (85 percent efficient). One of these has a further requirement that at least 90 percent of the material in the fine-size bin must pass the No. 10 sieve. The fifth agency requires that 90 percent of the material in a size-group must meet the nominal size requirements for the group, except that at least 95 percent of the material in the fine-size bin must pass the No. 10 sieve.

Four of the five agencies that limit only the undersize material in a size-group separate their aggregates into only two sizes, and place a limitation on the amount of fine material that may be carried into the coarse-size bin. One of the four reports that no carryover is allowed, one allows up to 8-percent carryover, and two allow up to 10-percent carryover. The fifth agency allows up to 10 percent undersize in the No. 2 bin (the No. 1 bin containing the finest-size aggregate), up to 15 percent undersize in the No. 3 bin, and up to 20 percent undersize in the No. 4 bin.

### Hot-Aggregate Bins

Either two, three or four compartments are required for separating the hot aggregates into size groups. As will be seen from Table 11-d, 7 agencies require at least two compartments for binder-course material, 33 agencies require 3 compartments, and 4 agencies require 4 compartments. Practice with regard to surface-course material will be noted in the table to be almost identical. Six agencies did not report for binder-course material, and four agencies did not report for surface-course material.

Capacity requirements for hot bins are also summarized in Table 11-d. Twelve agencies require only that the bin capacity be sufficient to supply the plant-rate, 7 require the bin capacity to be sufficient to supply the full capacity of the mixer, five re-

TABLE 11-d  
REQUIREMENTS FOR HOT-AGGREGATE BINS

Minimum Number of Compartments Required	Number of Agencies		Bin Capacity Required	Number of Agencies
	Binder Course	Surface Course		
2	7	8	Supply plant-rate	12
3	33	34	Supply full capacity of mixer	7
4	4	4	Not less than three times dead-load capacity of mixer	5
One for each aggregate size	1	1	Not less than ten times dead-load capacity of mixer	1
Not reported	5	3	Six-ton minimum capacity	1
			No requirement	10
			Not reported	14

TABLE 11-e

### THERMOMETRIC EQUIPMENT FOR AGGREGATES

Type of Instrument Permitted	No. of Agencies	Recording and Non-recording Instruments	No. of Agencies	Minimum Number of Instrument Terminals		No. of Agencies	Required Instrument Sensitivity and Efficiency	No. of Agencies
				Single Drier	Dual Drier			
Pyrometer and thermometer	43	Recording instrument required	25	1	2	11	Record 10° F. change in one minute	1
Pyrometer only	5	Non-recording instrument permitted	25	1	Dual not used	11	Record 10° F. change within 15 minutes	1
Not specified	2			1	1	6	Record 25° F. change within one minute	1
				2	3	1	Record 10° F. variation	1
				3	3	1	As directed	1
				4	5	1	Not specified	22
				Not specified		13	Not reported	24
				Not reported		6		



quire that the capacity be three times the dead-load capacity of the mixer, and one requires a capacity of not less than ten times the dead-load capacity of the mixer. One agency sets six tons as a minimum capacity. Ten agencies have no requirement, and 14 did not reply.

#### Thermometric Equipment for Aggregate

The replies that were received to several questions concerning thermometric equipment for measuring the temperature of hot aggregate are summarized in Table 11-e. It will be noted that 43 agencies will permit the use of either a pyrometer or thermometer, 5 require that a pyrometer only be used, and two do not specify. Twenty-five of the 50 reporting agencies require that recording instruments be used, while the other 25 permit the instruments to be non-recording.

Twenty-eight agencies use but one terminal on thermometric instruments when single driers are used. Eleven of these require two terminals when dual driers are used, but six do not. The remaining 11 do not use dual driers. Only three agencies appear to require additional terminals to be placed in the bins. One agency requires one additional terminal, one requires two additional terminals and one requires three additional terminals. This information is also summarized in Table 11-e.

Only four agencies indicate that they regulate within specific limits the sensitivity and efficiency of the thermometric instruments. Data concerning this item are also summarized in Table 11-e.

#### Storage Tank for Bituminous Material

Regulations concerning the capacity of the storage tank for bituminous material are summarized in Table 11-f. Of the 30 agencies reporting on their requirement, 20 report that they require only that the capacity be sufficient for one day's run. The various requirements of the other ten may be seen by referring to Table 11-f. Nineteen agencies reported that they do not specify a capacity for the tank for bituminous material.

#### Thermometric Equipment for Bituminous Material

Forty-six of the reporting agencies indicate that a thermometer is used for measuring the temperature of the bituminous material. Three of these indicate the additional use of a pyrometer, and three also indicate that a recording-type instrument is used. Four agencies did not indicate the type of thermometric equipment that is used.

### MIXING PLANTS

Forty-six of the reporting agencies permit the use of either batch-type or continuous-type mixers. The remaining four reporting agencies require the use of batch-type mixers. Twenty-three agencies use the batch-type mixer more frequently, and four use the continuous-type more frequently. Twenty-three agencies use both types with equal frequency. These data are tabulated in Table 11-g.

TABLE 11-g

USAGE OF BATCH-TYPE AND CONTINUOUS-TYPE MIXING PLANTS

Usage	Number of Agencies
Permit either batch-type or continuous-type mixers	46
Permit batch-type only	4
Use batch-type more frequently	23
Use continuous-type more frequently	4
Use both types with equal frequency	23

#### Batch-Type Mixing Plants

#### Aggregate Weighing Equipment

Information that was furnished by the

TABLE 11-f

REQUIRED CAPACITY OF TANK FOR BITUMINOUS MATERIAL

Tank Capacity Regulation	Number of Agencies
Sufficient for one day's run	20
Sufficient for continuous operation	4
In excess of plant operation	1
Sufficient for ten-hour operation	1
500 gal.	1
4,500 gal.	1
10,000 gal.	1
Two tanks for truck delivery	1
Not reported	1
Not specified	19

TABLE 11-h

## AGGREGATE WEIGHING EQUIPMENT FOR BATCH-TYPE PLANTS

Type of Scale Used	Number of Agencies	Required Scale Accuracy - Maximum Tolerance	Number of Agencies
Multiple beam, springless dial	37	0.5 percent of maximum load	16
		0.5 percent of load	14
Springless dial only	7	0.4 percent of maximum load	1
Type not indicated	6	0.4 percent of load	3
		± 2 lb	1
		± 5 lb	2
		± 20 lb.	1
		± 50 lb	1
		Based on scale graduation	2
		Other	1
		Approved	2
		Not specified	4
		Not reported	2

TABLE 11-i

## MEASURING BITUMINOUS MATERIAL IN BATCH-TYPE PLANTS

Method of Measurement	No. of Agencies	Type of Scales Used	No. of Agencies	Required Weigh-Bucket Capacity	No. of Agencies
By weight	50	Beam or springless dial	15	10 pct. of mixer capacity	4
By volume and weight	25	Springless dial	6	11 pct. of mixer capacity	1
		Beam	1	12 pct. of mixer capacity	2
		Spring-type	1	15 pct. of mixer capacity	3
		Springless dial or cylinder	1	20 pct. of mixer capacity	3
		Type not reported	26	25 pct. of mixer capacity	1
				10-20 pct. of mixer capacity	1
				15 pct. of aggregate wt	2
				20 pct. of aggregate wt	3
				Sufficient, adequate, etc	7
				Not specified	16
				Not reported	7

reporting agencies concerning aggregate-weighing equipment is tabulated in Table 11-h. As will be seen from the table, thirty-seven agencies state that they use either multiple-beam or springless-dial scales. Seven use the springless-dial scale only. Six agencies did not indicate the type used.

Regarding the required accuracy of the aggregate scales (see Table 11-h), 16 agencies report that they require an accuracy within 0.5 percent of the maximum load to be carried, and 14 report that they require an accuracy within 0.5 percent of the load carried. Considerable variation occurs in the practice reported by other agencies, as will be seen from the table.

### Measuring Equipment for Bituminous Material

Data regarding the measuring equipment for bituminous material in batch-type plants are summarized in Table 11-i. All agencies have plants operating using the weight method of measurement, and 25 have plants in which the bituminous material is metered by volume.

Regarding the type of scales used, 15 report using either beam or springless-dial scales, 6 report using the springless-dial type only, one reports using a beam scale only, and two report using other types (see Table 11-i). Twenty-six agencies did not report on scale type.

Twenty agencies reported specific requirements regarding the weigh-bucket capacity for bituminous material. These

requirements range from 10 percent to 25 percent of the mixer capacity, and from 10 to 20 percent of the aggregate weight. As will be seen from Table 11-i practice is well divided through these ranges. Seven agencies require that the capacity be sufficient, adequate, etc., 16 reported that they have no specification requirement, and 7 did not report.

### Batch-Type Mixers

A number of questions were asked concerning specification requirements for, and usage of, batch-type mixers. Several of the questions were concerned with detailed items which many agencies appear not to cover directly in their specifications. Such replies as were received are summarized in Table 11-j, and are discussed in the following paragraphs.

Forty-seven of the reporting agencies use twin-shaft mixers exclusively. Only two report that some use is made of rotary-drum mixers in addition to the twin-shaft mixer.

Regarding permissible minimum mixer capacity, a variety of replies were received (see table). Of 25 agencies that report having a minimum capacity requirement (that is, in pounds per batch), 16 have set a 2,000-lb minimum, 4 have a 1,500-lb minimum, 4 have a 1,000 lb minimum, and 1 agency has a 750-lb minimum. Such other capacity requirements as were reported will be seen by referring to the table. Fifteen agencies report that they do not specify a minimum capacity, and four did not report.

TABLE 11-j  
USAGE AND REQUIREMENTS-BATCH-TYPE MIXERS

Type of Mixer Normally Used	Number of Agencies	Permissible Minimum Mixer Capacity	Number of Agencies	Mixer-Blade Rotation Rate rpm	Number of Agencies	Maximum Allowable Blade Clearance inches	Number of Agencies
Twin shaft	47	750 lbs.	1	40	1	1/2	1
Rotary drum or twin shaft	2	1000 lbs.	4	40-60	1	3/4	18
Not reported	1	1500 lbs.	4	56	1	1	2
		2000 lbs.	16	55-75	1	1-1 1/2	1
		300 ton/8 hrs.	1	58-60	1	2	8
		52 cu. ft.	1	60+	2	Not specified	14
		Rated capacity	2	70-90	2	Not reported	6
		1/2 rated capacity	1	Mfgr's. rate	3		
		Depends on job	1	For uniform mix, etc.	2		
		Not specified	15	Not reported	36		
		Not reported	4				

Time Lock	Number of Agencies	Specified Minimum Lock Interval seconds	Number of Agencies
Use time lock	26	2	1
Do not use time lock	24	5	10
		10	1
		15	1
		Not specified	6
		Not reported	31

TABLE 11-k  
USAGE AND REQUIREMENTS-CONTINUOUS-TYPE MIXERS

Type of Mixer Normally Used	Number of Agencies	Usual Maximum Rate of Production tons per hour	Number of Agencies	Angular Adjustment Required for Paddles	Number of Agencies	Paddles Required Capable of Reverse Motion	Number of Agencies	Minimum Allowable Capacity of Discharge Hopper lbs.	Number of Agencies
Twin pugmill	41	40	1	Angular adjustment required	40	Reverse motion required	27	2000	5
Twin or single pugmill	2	50	2	Angular adjustment not required	2	Reverse motion not required	15	1000	1
Not reported	3	120	4	Not reported	4	Not reported	4	One batch	1
Type not used	4	125	1	Type not used	4	Type not used	4	Not specified	27
		160	1					Not reported	12
		80 min.	1					Type not used	4
		40-120	1						
		80-100	1						
		Not reported	34						
		Type not used	4						

Only nine agencies reported on the rotation rates of the mixer blades of the mixers used on their construction projects. Reported rates vary from 40 to 90 rpm (see table).

Thirty agencies reported on their specifications regarding mixer-blade clearance. Fourteen agencies report that they have no specifications regarding this particular item, and six did not report. Of the 30 agencies reporting a specification, 18 have established  $\frac{3}{4}$  in. as a maximum clearance, and 8 have established 2 in. Maximum clearances permitted by the remaining four agencies will be seen by referring to Table 11-j.

Twenty-six of the 50 reporting agencies report that a time lock is used on their mixers. The remaining 24 do not use a time lock. Thirteen of the agencies report that they have specifications covering a minimum lock interval. Ten of these have set a minimum interval of 5 seconds, 1 requires 2 seconds, 1 requires 10 seconds, and 1 requires 15 seconds.

### Continuous-Type Mixing Plants

#### Continuous-Type Mixers

Several questions similar to those that were asked concerning batch-type mixers were asked concerning continuous-type mixers. The replies are summarized in Table 11-k, and are discussed in the following paragraphs.

Of the 46 agencies using continuous mixers, 41 report that usage is confined to the twin-pugmill mixer. Two agencies report that they use a single-pugmill mixer in addition, and three agencies did not report.

Only twelve agencies reported on the usual maximum rate of production. Reported rates vary from 40 to 160 tons per hour. Four agencies report a maximum rate of 120 tons per hour, and, as will be seen from the table, the rates reported by the other agencies are well distributed through the range of 40 to 160.

Of 42 agencies reporting concerning a requirement for angular adjustment of the mixer paddles, 40 report that they require the paddles to be capable of angular adjustment, and two report that angular adjustment is not required.

Of 42 agencies reporting concerning a requirement that the paddles be capable of reverse motion, 27 report that this is required. The remaining 15 report that reverse motion is not required.

Only six of the 46 agencies using continuous mixers report that they specify a minimum allowable capacity for the discharge hopper of the pugmill. Five of these require a minimum capacity of 2,000 lb of mixture, and one requires a minimum capacity of 1,000 lb.

### TRANSPORTATION

Forty-one of the 50 reporting agencies state that a cover for the material is required during transportation from the mixing plant to the road-site. Six additional agencies indicate that a cover is used when one is considered to be needed, particularly in cool weather. Only three agencies report that no cover is required. Of the agencies answering the question as to the type of cover specified, all indicate the use of a cloth cover. Such terms as "canvas," "waterproof canvas," and "tarpaulin" were used, but it is believed that all refer to the same type of material. One agency indicates permitting the use of heavy paper as well as canvas.

Only seven agencies indicate that they require regular use of body insulation on trucks transporting bituminous-concrete mixtures. Seven additional agencies indicate that insulation is required occasionally, particularly in cool weather or during long hauls. Only two agencies reported on the type of insulation specified; one requiring wood and the other celotex. Two agencies report requiring a  $\frac{3}{4}$ -in. thickness of insulation without mentioning

TABLE 11-1  
SPREADING AND FINISHING MACHINE

Use of Side Forms	Number of Agencies	Use of Leveling Device	Number of Agencies	Use of Scribed Heater	Number of Agencies
Not used	45	Used	31	Used	45
Required	2	Not used	15	Not required	2
Optional	2	Optional	1	Not specified	1
Not reported	1	Not reported	3	Not reported	2

TABLE 11-m

REQUIREMENTS FOR COMPACTING ROLLERS<sup>1/</sup>

Specified Total Weight Limit Tons	Number of Agencies	Specified Compression Weight lb per in. roller width	Number of Agencies
<u>Tandem</u>		<u>Tandem</u>	
5-8	1	200	7
5-10	2	200+	4
6	1	250	5
6-10	1	200-250	1
7	1	250	6
7-10	4	250+	5
8	2	250-400	1
8+	7	250+	1
8-10	7	300+	1
8-12	9	325	2
10	2	330	1
10+	4	Not specified	13
10-12	1	Not reported	6
10-14	2		
Not specified	3	<u>Three Wheel</u>	
Not reported	1	200	7
		200+	4
<u>Three Wheel</u>		250	4
5-10	2	250+	2
7-10	1	250-400	1
8	2	300	1
8-10	2	300+	1
8-12	5	310-350	1
10	10	325	2
10+	4	330	2
10-12	5	350	1
10-14	2	Not specified	9
Not specified	4	Not reported	3
Not reported	1		
<u>Pneumatic</u>		<u>Pneumatic</u>	
8-10	1	250	1
10	1	325	2
10-14	2	Not specified	4
Not specified	1		
<u>Three-Axle Tandem</u>		<u>Three-Axle Tandem</u>	
12-19	1		
16-21	1		

<sup>1/</sup> Summary information on roller-type requirements is presented in Table 10-1.

were previously discussed, and summary information was reported in Table 10-1. Information on specified weight limits for rollers, and specified compression weights, is now summarized in Table 11-m. An inspection of the table will show that, except for three-axle tandem rollers, most agencies require total weights of from 8 to 12 tons, with a scattering of agencies permitting rollers weighing as little as 5 tons and as much as 14 tons. Of two agencies specifying total weights for three-axle tandem rollers, one specifies a range of from 12 to 19 tons, and the other a range of from 16 to 21 tons. Specified compression weights of from 200 to 250 lb per in. of roller width are usually required, with a few requiring somewhat higher compression weights. One permits a compression weight of up to 400 lb per in. of roller width.

### TESTS OF MIXTURES

The cooperating agencies were asked to report on the various tests that are made on samples taken from regularly-produced paving mixtures. They were also asked to indicate which tests are performed in field laboratories, and which are performed in central laboratories; and which are made on samples taken from trucks or at discharge from the mixer, and which are made on samples taken from the compacted pavement.

Of 40 agencies reporting on the frequency with which samples are taken from the compacted pavement to determine in-place density, at least eighteen indicate that they take about one sample a day minimum. One agency reports taking two per day, and another four per day. One agency reports taking one every other day. Several other agencies reporting on a tonnage or sq yd basis indicate a similar frequency of sampling. Five agencies report that samples are taken rarely, occasionally, etc., and two report that sampling frequency is at the Engineer's discretion. Only four agencies report that samples are not taken from the compacted pavement. Hand tools, core drills, air hammers, and saws are most frequently used for the removal of samples from the compacted pavement.

### TESTS IN FIELD LABORATORY

The information that was received regarding tests made in field laboratories on

type, and one agency reports requiring a 1/2-in. thickness without mentioning type.

### SPREADING AND FINISHING MACHINE

A very limited number of questions were asked concerning spreading and finishing machines. The information that was received is summarized in Table 11-1. In reply to a question as to whether side forms are used, two report that they are required, and two report that the use of side forms is optional. Concerning the use of a leveling device to compensate for irregularities in the surface upon which the bituminous material is being placed, 31 agencies report the use of such a device, 15 report that such a device is not used, and 1 reports that the use of such a device is optional. Regarding the use of screed heaters, 45 agencies report that a screed heater is used, and 3 agencies report that the use of a screed heater is either not required or not specified.

### COMPACTING ROLLERS

TABLE 12-a  
TESTS PERFORMED IN FIELD LABORATORY ON SAMPLES OF  
PLANT-PREPARED BITUMINOUS-CONCRETE MIXTURES

Test	Total Number of Agencies Making Test in Field Laboratory	Number of Agencies Making Test in Field Laboratory on Sample of:		
		Loose Mixture	Compacted Pavement	Undetermined
Gradation	46	38	16	1
Extraction	35	26	14	2
Density <sup>1/</sup>	29	5	28	0
Marshall	8	5	2	1
Hubbard-Field	1	1	0	0
Thickness	2	0	2	0
Moisture Content	1	1	0	0
Compaction	1	1	0	0

<sup>1/</sup> Many agencies calculate the theoretical void content following the determination of density of samples from the compacted pavement.

TABLE 12-b  
TESTS PERFORMED IN CENTRAL LABORATORY ON SAMPLES OF  
PLANT-PREPARED BITUMINOUS-CONCRETE MIXTURES

Test	Total Number of Agencies Making Test in Central Laboratory	Number of Agencies Making Test in Central Laboratory on Sample of:		
		Loose Mixture	Compacted Pavement	Undetermined
Gradation	36	30	16	0
Extraction	45	37	19	1
Density <sup>1/</sup>	29	7	28	0
Marshall	12	9	4	0
Hveem Stabilometer	8	6	3	0
Hubbard-Field	5	3	2	0
Triaxial Compression	2	1	1	0
Unconfined Compression	2	0	0	2
Hveem Cohesimeter	2	2	1	0
Abson Recovery	4	1	4	0
Swell	2	1	1	0
Thickness	4	0	4	0
Moisture Content	1	1	0	0
Compaction	1	1	0	0

<sup>1/</sup> Many agencies calculate the theoretical void content following the determination of density of samples from the compacted pavement.

mixture samples is summarized in Table 12-a. It will be noted from the table that tests most frequently made on samples of loose material and also on samples of the compacted pavement are gradation, extraction, and density tests. Forty-six agencies indicate that gradation tests are made in a field laboratory, 35 indicate that extraction tests are made in the field, and 29 indicate that density tests are made in the field. As would be expected, gradation and extraction tests are more frequently made on samples taken from the loose mixture rather than from the compacted pavement. Twenty-eight of the 29 agencies making density tests determine the density of specimens taken from the compacted pavement. Four of these also conduct density (or compaction) tests on samples taken from the loose mixture. One agency makes density (compaction) tests only of samples taken from the loose mixture. Additional details of practice will be seen by referring to Table 12-a.

### TESTS IN CENTRAL LABORATORY

Table 12-b contains data similar to that contained in Table 12-a, except that the data relate to tests performed in the central laboratory. Fewer agencies perform gradation tests on field-obtained samples in the central laboratory than perform these tests in the field laboratory (36 as compared with 46). A greater number perform extraction tests in the central laboratory (45 as compared with 35). An equal number (29) perform density tests in the central laboratory and in the field.

The Marshall and Hubbard-Field tests are made much more frequently in the central laboratory, and the Hveem, triaxial, and unconfined compression tests are made only in the central laboratory. Details regarding the number of agencies performing these and other tests of samples obtained in the field will be found in Table 12-b.

A further comparison of practice regarding central and field laboratory testing of field-obtained samples is presented in Table 12-c for the three principal tests. It will be seen that the gradation test is used by all but one of the 50 reporting agencies, and that samples are tested in both field and central laboratories by 33 of the agencies. Thirteen of the agencies use the gradation test in the field only, and 3 use the test in the central laboratory only. It will also be seen from the table that all agencies make use of the extraction test, 30 using the test in both field and central laboratories. Five agencies use the test in the field only, and 15 use the test in the central laboratory only. Continuing to refer to Table 12-c, it will be seen that 40 of the 50 reporting agencies make use of the density test on field-obtained samples. Seventeen use the test in both field and central laboratories, 11 use the test in the field only, and 12 use the test in the central laboratory only.

## Appendix I

### PRIME COAT

Questionnaire returns indicate that all but two of the reporting agencies apply a coating of asphalt or tar to the base that is to receive the asphaltic concrete. The term "prime coat" is applied to this coating most frequently when a granular base is involved and some penetration is expected. The term "tack coat" is frequently used when the bituminous material is applied to a concrete base. The term "bond coat" is also sometimes used. Terminology is not consistent; and since the term "prime coat" was the only one used on the questionnaires some of those who filled in the replies may have met with some difficulty in understanding the answers that were desired. However, it is not believed that the confusion was sufficient to seriously affect the reliability of the answers.

The more important features of the returns are summarized and discussed in the paragraphs which follow. Details of the replies that were received are tabulated in Appendix Table 13.

TABLE 12-c  
SUMMARY DATA REGARDING PRINCIPAL TESTS  
PERFORMED ON FIELD-OBTAINED SAMPLES IN  
FIELD AND CENTRAL LABORATORIES

	Number of Agencies Conducting Test		
	Gradation	Extraction	Density
Test made in field laboratory only	13	5	11
Test made in central laboratory only	3	15	12
Test made in both field and central laboratories	33	30	17
Test not used	1	-	10
Total agencies reporting	50	50	50

## BITUMINOUS MATERIAL

The reporting agencies were asked to list the grades of asphalt and tar that they use for priming bases upon which is to be placed bituminous concrete, and to indicate the type and grade of material that is normally used on flexible base, and on rigid base. Forty-eight of the agencies make at least some use of asphalt, and 20 make at least some use of tar. Two agencies do not use a prime coat. A summary of the information that was furnished by the agencies concerning the specific types and grades of asphalts and tars normally used is presented in Table 13-a. It will be noted from the table that Type MC and Type RC asphalts are used most frequently on flexible bases (Type MC by 21 and Type RC by 7 of 30 reporting agencies). Type RC and emulsified asphalts are the types most frequently used on rigid bases (Type RC by 20 and emulsified asphalts by 9 of 27 reporting agencies). Individual grades of asphalt used most frequently are Grades MC-1 and MC-0 for flexible bases (by 12 and 8 agencies respectively), and Grades RC-1 and RC-0 for rigid bases (by 9 and 7 agencies respectively).

Agencies using tar as a prime-coat material confine its use almost wholly to flexible base (one exception). For agencies reporting on the grade of tar used (only five reported grade), three use RT-2, three use RT-3 and two use RT-1. All of this usage is on flexible base.

Specifications controlling the characteristics of the various grades of bituminous material are, for most of the reporting agencies, identical with specifications recommended by the AASHO. The few variations that do occur are mostly of a minor nature. Where a spot requirement is listed by the AASHO as optional, ten agencies report definitely that they do not have a spot-test requirement. Twelve agencies indicate that a negative spot is required when the test is made with standard naphtha solvent; five indicate that a negative spot is required with 35 percent heptane xylene solvent; three require a negative spot with 15 percent naphtha xylene solvent; and two require a negative spot with 10 percent naphtha xylene solvent.

## CONSTRUCTION PRACTICE

### Application Rate

Forty-three agencies reported on the unit quantities of bituminous material applied to flexible bases. The over-all limits of application reported range from 0.10 to 0.60 gal per sq yd. Only 14 percent of the agencies indicate that applications of less than 0.15 or more than 0.50 gal per sq yd are made.

Thirty-six agencies reported on the unit quantities of bituminous material applied to rigid bases. The over-all limits of application reported range from 0.02 to 0.50 (?) gal per sq yd. Only 19 percent of the agencies indicate that applications of less than 0.03 or more than 0.15 gal per sq yd are made.

A tachometer is used by all but one of the reporting agencies in determining the rate of application of the bituminous material. The agency not using a tachometer reports that distances through which the distributor is to travel are measured and that this measurement is used in determining the rate of application. Two of the agencies using a tachometer also report the use of a synchronizer.

TABLE 13-a

TYPES AND GRADES OF BITUMINOUS MATERIAL NORMALLY USED FOR PRIME COAT OF BASE ON WHICH IS PLACED BITUMINOUS CONCRETE

Type and Grade of Bituminous Material	Number of Agencies Normally Using Type and Grade On Flexible Base	On Rigid Base
<u>Type RC asphalt</u>	7	20
Grade RC-0	1	7
RC-1	5	9
RC-2	2	5
RC-3	2	2
RC-4	1	1
<u>Type MC asphalt</u>	21	4
Grade MC-0	8	3
MC-1	12	2
MC-2	5	1
<u>Type SC asphalt</u>	1	
Grade SC-2	1	
<u>Emulsified asphalt</u>	1	9
Type AEM-1		1
AE-2		1
AE-5		1
AE-7	1	1
MS-1		5
MS-2		1
<u>Tar</u>	5	
Grade RT-1	2	
RT-2	3	
RT-3	3	
RT-4	1	
<u>DNO Asphalt Primer (Ont)</u> <sup>1/</sup>	1	1
Total agencies reporting	30	27
Agencies reporting normal use of more than one type and grade of material	9	3

<sup>1/</sup> Resembles Type RC



## Application Temperature

A question was asked concerning the temperature at which bituminous priming materials are applied, but space was not provided on the questionnaires for indicating the grades of material to which the reported application temperatures applied. The variety of answers that were received seem to indicate that the method of replying to this question was not uniform, so no summary has been made of the information that was received. Over-all, the reported material temperatures at application vary from 50 F to 225 F. About one-third of the 37 agencies reporting application temperatures indicated temperatures that can be reached in normal summer weather without heating. The remainder indicated temperatures likely to be reached only through heating. As would be expected, the agencies using the higher grades of asphalt reported the higher application temperatures.

## Curing Period

Only 16 of 41 agencies specify a fixed minimum curing period. The remainder either do not specify a curing period, or include in their specifications a general statement that curing shall be continued until the prime is "properly cured," "tacky," "blotted," etc. Of the 16 agencies specifying a fixed minimum curing period, 8 specify a minimum period of 25 hr. Other minimum periods reported vary from 1 hr to 7 days.

## *Appendix II*

### THICKNESS OF PAVEMENTS SURFACED WITH BITUMINOUS CONCRETE

In an effort to assemble some information on the thicknesses of flexible pavement that the reporting agencies would be likely to use under the conditions that prevail in the area of the Test Road, they were asked to indicate the thicknesses of the various pavement components that they would be likely to use if they were to design a pavement for the area. The natural soil was listed as an A-6 soil, the average annual rainfall was stated to be 32 in., and the average annual frost penetration was listed at 28 in. Agencies were asked to indicate the method of flexible pavement design that they use, and whether or not the character of the subgrade soil is taken into consideration in their method of design. They were also asked to furnish designs for medium and heavy traffic, providing their methods took traffic into consideration.

## Design Methods

Since it was desired that the reporting agencies indicate the thicknesses of pavement they would be likely to use under the conditions of the area of the Test Road, it was also considered desirable to obtain general information on the method by which they arrive at pavement thickness. However, it was considered beyond the scope of the questionnaires to cover thoroughly the broad and complex subject of thickness design, and as a consequence, the information that was obtained is very limited and in some instances probably not very precise.

In Table 14-a are summarized the replies that were received concerning the

TABLE 14-a  
SUMMARY OF REPORTED METHODS OF DESIGN  
OF FLEXIBLE PAVEMENT THICKNESS

Design Method	Number of Agencies	Design Method	Number of Agencies
Past experience	9	HRB Group Index, traffic, rainfall, and drainage	1
HRB Soil Classification	3	Traffic, rainfall, gradation, and Atterberg limits of base and subbase material	1
CBR (modified)	3	Traffic and bearing value	1
CBR	2	Triaxial	1
Hveem Stability Test	2	Triaxial-modified Hveem	1
Volume and type of traffic	2	Traffic volume and soil type	1
California Method	1	Gradation and plate bearing tests	1
Colorado Method	1	Rational determination	1
Hveem Method	1		
Kansas Triaxial Method	1	Total	12
North Dakota Method	1		
P I of subgrade soil and amount of minus No. 200 sieve material	1		
CBR and frost penetration	1		
CBR and HRB Soil Class	1		
CBR (modified) and Hveem Stability Test	1		
Ky (CBR) and Ohio (HRB) design curves	1		
HRB Soil Class, traffic, drainage and frost penetration	1		
HRB Soil Class and traffic	1		
Soil profile and estimated stability of foundation	1		

method used to determine the thickness of flexible pavements. It will be seen that the replies vary widely, and that many were not sufficiently complete to indicate the overall design procedure. For example, a number of agencies indicate only a physical test that is used as part of the design procedure. However, there is a definite indication that most agencies attempt to evaluate one or more of the conditions that must be satisfied before the pavement structure can be expected to serve adequately, and to vary the thickness accordingly.

Subgrade Character in Design

The agencies were asked to indicate the manner in which subgrade soil characteristics are taken into consideration in their designs for pavement thickness. Replies that were received are summarized in Table 14-b. It will again be seen that there was a considerable variation in the methods of replying to the question and that the information that was received is not complete. However, it is evident that almost all agencies give consideration to subgrade conditions and the character of the subgrade soil in selecting pavement thickness.

Pavement Thickness

As mentioned previously, the reporting agencies were asked to determine the total pavement thickness and also the thickness of the individual components that their design procedures would indicate to be satisfactory under the following conditions:

Subgrade soil class	A-6
Average annual rainfall	32 in.
Average annual frost penetration	28 in.

Designs were to be furnished for pavements consisting of bituminous concrete placed on both flexible (granular) and rigid bases overlying granular subbases. The agencies using design procedures that take traffic into account were asked to furnish designs for "medium" and "heavy" traffic. Twenty-seven agencies furnished complete thickness designs for heavy-traffic flexible pavement, 28 for medium-traffic, and 10 for flexible pavement without differentiating as to traffic.

TABLE 14-b  
SUMMARY OF REPORTED USE OF SUBGRADE SOIL CHARACTERISTICS  
IN DETERMINING THE THICKNESS OF FLEXIBLE PAVEMENTS

Characteristics Evaluated	Number of Agencies	Characteristics Evaluated	Number of Agencies
IRS Soil Class	5 (1)1/	Nveem stabilometer test value and swell pressure	1
CBR	6 (2)	CBR (modified), Nveem stabilometer test value, and frost reaction	1
Subgrade soil type	3 (2)	Past experience	1
Bearing value or ability	3		
Subgrade soil characteristics	4 (2)1/	Total	40
ECI Group Index	2		
Drainability	2		
IRS Soil Class and CBR	2		
Not evaluated	2		
PI and amount of minus to 200 sieve material	1		
Shearing resistance and expansive characteristics	1		
CBR (modified)	1		
Nveem method	1		
Modulus of deformation from triaxial test	1		
Mechanical analysis and plate-bearing value	1		
Soil type and max. comp. value	1 (1)		
Stabilometer value and silt content	1		
Shear strength, triaxial test	1		

1/ Numbers in parentheses indicate the number of agencies stating that variations are made in only the subbase thickness as a result of the evaluation of subgrade soil characteristics

2/ On agency states that both base and subbase thickness are varied on the basis of the evaluation of subgrade soil characteristics

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS		
Granular subbase and base, bituminous concrete surface		
Subgrade soil class		
Average annual rainfall		
Average annual frost penetration		
A-6		
32 in		
28 in		

TABLE 14-c SUMMARY OF TOTAL PAVEMENT THICKNESSES LIKELY TO BE USED BY THE REPORTING AGENCIES UNDER THE FOLLOWING		
---	--	--

Only 11 agencies furnished complete thickness designs for rigid-base pavement.

**Total Thickness-Flexible Base.** The total-thickness figures that were reported for the flexible-base pavement are summarized in Table 14-c. It will be noted that almost as many different thickness figures were reported as there were agencies reporting. The figures for total thickness that were reported range from 5 to 27 in. for the agencies that do not make a distinction on the basis of traffic; from 8 to 39 in. for heavy-traffic pavements; and from 5 to 38½ in. for medium-traffic pavements for agencies that take traffic into consideration in their design procedures. About three-quarters of the agencies reporting thickness designs without considering traffic listed figures within the limits of 11½ and 19 in.; about three-quarters of those reporting for heavy-traffic pavements listed figures within the limits of 14 and 29 in.; and about three-quarters of those reporting for medium-traffic pavements listed figures within the limits of 9 and 25½ in.

It is not believed that the wide variation in thickness as determined by the different design procedures in use is attributable entirely to differences in the procedures. It is known, for example, that the information that was given concerning the subgrade soil was insufficient for many agencies (although it was all that was available at the time), and additional assumptions had to be made before many of the design procedures could be applied. Additional assumptions would be expected to cause a spread in the results. Other assumptions that were necessary, such as a more precise defining of the terms "heavy traffic" and "medium traffic," and perhaps in some instances the extrapolation in procedures not developed to cover the specified conditions of rainfall and frost, could be expected to cause further variation in results. The fact that many of the agencies chose to report ranges in thickness rather than a specific thickness is a good indication that they considered the information that was given as being insufficient for designing by their procedures.

A comparison of the ratios of the bituminous concrete surfacing to the total thickness for each agency did not indicate that the thickness of the surfacing had any consistent influence on total thickness.

**Granular Subbase and Base Thickness.** The granular subbase and base thicknesses determined by the reporting agencies for use with a bituminous-concrete surfacing under the conditions of soil, climate and traffic that have previously been listed are summarized in Table 14-d. It will be noted that here again the thicknesses determined by the different procedures used by the reporting agencies vary considerably. The agencies are, however, in better agreement on base thickness than on either subbase thickness or total pavement thickness.

The reported subbase thicknesses range from 0 to 18 in. and average 8.3 in. where no differentiation is made as to traffic. For heavy-traffic pavements, the reported subbase thicknesses range from 0 to 36 in. and average 11.8 in. For medium-traffic pavements, the reported subbase thicknesses range from 0 to 24 in. and average 9.8 in.

Reported base thicknesses range from 2 to 10 in. and average 5.4 where no differentiation is made as to traffic. For heavy-traffic pavements, the base thicknesses range from 2 to 24 in. and average 8.0 in. For medium traffic pavements, reported thicknesses range from 2 to 18 in. and average 6.4 in.

**Bituminous-Concrete Thickness (Flexible Base).** Much better agreement prevails

TABLE 14-d  
SUMMARY OF GRANULAR SUBBASE AND BASE THICKNESSES LIKELY TO BE USED  
BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS

	Bituminous concrete surface		A-6	
	Subgrade soil class		3c in	
	Average annual rainfall		3d in	
	Average annual frost penetration		2d in	
	<u>Thickness Reported 1/</u>			
No Traffic	Heavy-Traffic		Medium-Traffic	
Differentiation	Pavement		Pavement	
	<u>SUBBASE</u>			
inches	inches	inches	inches	inches
0-13	0-6	9 (2)	0-10	9
4-6	0-12	10	0-12	10
4-12	0-18	10½	0-13	12 (3)
6 (2)	3-13	12 (2)	0-16	12-14
6-18	4	12-18	3	12-15
8	5+	12-20	4-6	14½
11	6-9	13	5	15
12 (2)	6-10	15	6	18
	7	17	6-9	18-24
	8	18-20	6-12	
	8-12	20	6-15	
		24	7 (2)	
		24-36	8	
			8-12	
Overall range 0-18 in	Overall range 0-36 in		Overall range 0-24 in	
Average 8.3 in	Average 11.8 in		Average 9.8 in	
Total agencies 11	Total agencies 26		Total agencies 26	
	<u>BASE</u>			
2 (2)	2	6-10	2 (2)	6-10
2-10	3 (3)	7	3 (3)	7 (2)
3	3-6	8 (4)	4 (3)	7-10
4-8	4 (3)	9+	4-5½	7-12
4+	4½	10 (3)	4-6 (2)	8 (3)
5-10	5-6½	10-14	5-8	8-10
6 (2)	5-12	12 (2)	5½-6	9
8 (3)	5-18	12-21	6 (5)	18
	6 (3)	24		
Overall range 2-10 in	Overall range 2-24 in		Overall range 2-18 in	
Average 5.4 in	Average 8.0 in		Average 6.4 in	
Total agencies 12	Total agencies 30		Total agencies 29	

1/ Most of the thicknesses that are listed were reported by only one agency. Where more than one agency reported identical thicknesses, the number of agencies reporting appears in parentheses following the thickness figure.

1/ Most of the thicknesses that are listed were reported by only one agency. Where more than one agency reported identical thicknesses, the number of agencies reporting appears in parentheses following the thickness figure.

among the reporting agencies as to the thickness of bituminous concrete that should be used under the conditions of soil, traffic and climate that were specified. This will be seen from an inspection of Table 14-e where the reported data are summarized.

Reported total thicknesses for the bituminous surfacing range from  $2\frac{1}{2}$  to  $5\frac{1}{2}$  in.

TABLE 14-e

SUMMARY OF BITUMINOUS CONCRETE THICKNESSES LIKELY TO BE USED  
BY THE REPORTING AGENCIES UNDER THE FOLLOWING CONDITIONS

Bituminous concrete surface, granular base and subbase  
Subgrade soil class A-6  
Average annual rainfall 32 in.  
Average annual frost penetration 28 in.

No Traffic Differentiation	Thickness Reported 1/	
	Heavy-Traffic Pavements	Medium-Traffic Pavements
TOTAL THICKNESS OF BITUMINOUS CONCRETE		
inches	inches	inches
$2\frac{1}{2}$ (3)	1	1-3
$2\frac{1}{2}$ - $3\frac{1}{2}$	2 (2)	2 (5)
3 (2)	$2\frac{1}{2}$ (5)	$2\frac{1}{2}$ (9)
$3\frac{1}{2}$	$2\frac{1}{2}$ -3	3 (9)
4 (4)	3 (14)	$3\frac{1}{4}$
$5\frac{1}{2}$	$3\frac{1}{4}$	$3\frac{1}{2}$ (2)
	$3\frac{1}{2}$	$3\frac{1}{2}$ - $5\frac{1}{2}$
	4	
	$4\frac{1}{2}$	
	5	
Overall range $2\frac{1}{2}$ - $5\frac{1}{2}$ in.	Overall range 1-5 in.	Overall range 1- $5\frac{1}{2}$ in.
Average 3.5 in.	Average 3.0 in.	Average 2.7 in.
Total agencies 12	Total agencies 28	Total agencies 29
THICKNESS OF BINDER COURSE 2/		
1- $1\frac{1}{2}$	1	0-2
$1\frac{1}{4}$	$1\frac{1}{4}$ (2)	1 (2)
$1\frac{1}{2}$ (3)	$1\frac{1}{2}$ (9)	$1\frac{1}{4}$ (3)
2 (3)	1.7	$1\frac{1}{2}$ (9)
$2\frac{1}{2}$ (2)	1 $\frac{3}{4}$	1 $\frac{3}{4}$
4	2 (6)	2 (5)
	3	2-4
	$3\frac{1}{2}$	
Overall range 1-4 in.	Overall range 1- $3\frac{1}{2}$ in.	Overall range 1-4
Average 2.0 in.	Average 1.8 in.	Average 1.6
Total agencies	Total agencies 22	Total agencies 22
THICKNESS OF SURFACE COURSE 2/		
1	1 (5)	1 (8)
$1\frac{1}{4}$	1- $1\frac{1}{2}$	$1\frac{1}{4}$ (5)
$1\frac{1}{2}$ (6)	$1\frac{1}{4}$ (4)	$1\frac{1}{2}$ (9)
$1\frac{1}{2}$ -2	1.3	
2 (2)	$1\frac{1}{2}$ (10)	
Overall range 1-2 in.	Overall range 1-2 in.	Overall range 1- $1\frac{1}{2}$ in.
Average 1.6 in.	Average 1.4 in.	Average 1.3 in.
Total agencies 11	Total agencies 22	Total agencies 22
1/ Many of the thicknesses that are listed were reported by only one agency. Where more than one agency reported identical thicknesses, the number of agencies reporting appears in parentheses following the thickness figure.		
2/ The binder-course and surface-course thicknesses that are listed are for the agencies that reported thicknesses for both. Six agencies reported surface thickness only, and these are tabulated as total thickness.		

and average 3.5 in. where no differentiation is made as to traffic. For heavy-traffic pavements the range is from 1 to 5 in. and the average 3.0 in.; and for medium-traffic pavements the range is from 1 to  $5\frac{1}{2}$  in. and the average is 2.7 in. The over-all ranges are relatively great. However, an inspection of the table will show that a majority of the agencies suggest thicknesses within the range of  $2\frac{1}{2}$  to 3 in., regardless of traffic considerations, and that only a scattering of agencies suggest thicknesses at or near the extreme limits of the over-all ranges.

Table 14-e also contains a summarization of recommended binder-course and surface-course thicknesses. It will be seen that here again good agreement exists, and that the pattern is very much the same as that described for the total thickness of bituminous surfacing. The averages of the reported surface-course thicknesses for the different conditions of traffic range from 0.3 to 0.4 in. less than the averages of the reported binder-course thicknesses.

**Rigid-Base Pavement Thickness.** Only 11 agencies furnished thickness designs for pavements consisting of bituminous concrete placed on a rigid base (and, in most of the designs furnished, including a subbase). The conditions of soils, traffic and climate that were to be considered in preparing the design are the same as those set up for the flexible-pavement design. Six of the 11 agencies furnished separate designs for heavy- and medium-traffic pavements, and two furnished designs for heavy-traffic pavements only. The other three furnished designs without differentiating as to traffic, except that one of the three indicated that subbase would be omitted from the design under conditions of medium traffic.

The proposed over-all thicknesses range from 11 in. to 23 in. for designs for heavy-traffic pavements, from  $8\frac{1}{2}$  in. to 22 in. for designs for medium-traffic pavements, and from 10 in. to 23 in. where no traffic differentiation was made.

Subbases were proposed for use by 7 of 8 agencies furnishing heavy-traffic designs, by 6 of 9 agencies furnishing medium-traffic designs, and by 2 of 3 agencies not differentiating as to traffic. Two of the agencies furnishing both heavy- and medium-traffic designs reduced the subbase thickness by  $2\frac{1}{2}$  in. for the medium-traffic design, and a third agency proposed a subbase for heavy traffic but dispensed with the subbase for medium traffic. Otherwise, there is little discernible difference in the proposed subbase thicknesses insofar as traffic conditions are concerned.

Suggested thicknesses for the rigid base range from 4 in. to 10 in. The recommendations of all but 3 of the agencies are within the range of 6 to 8 in. Two agencies that recommend an 8-in. thickness of rigid base for heavy-traffic pavements reduce the thickness to 6 in. for medium-traffic pavements. The single agency that recommends a 10-in. rigid base for heavy-traffic pavements recommends 9 in. for medium-traffic pavements. Otherwise, there is little difference in the recommended rigid-base thicknesses with respect to traffic.

Proposed thicknesses for the bituminous-concrete surfacing for use with rigid base range from 1 in. to 3 in. Six of 8 agencies furnishing a heavy-traffic design propose the 3-in. thickness. One of these would reduce the thickness to  $2\frac{1}{2}$  in., and another to 2 in., for medium traffic. Only one agency recommended a 1-in. thickness of bituminous concrete, but made this recommendation for both heavy and medium traffic. Thicknesses of  $2\frac{1}{2}$  in. and  $2\frac{1}{4}$  in. were each recommended by one agency.

Only 8 agencies furnished complete thickness designs for both flexible base and rigid-base pavements. Thickness differentials ranging from 1 in. to 16 in. in favor of the rigid-base pavement were indicated in the designs of 6 of the agencies. One agency indicated the same thickness for both types of pavement, and one indicated a 1-in. differential in favor of the flexible pavement. Because of the few agencies that furnished information for this comparison, not much significance can be attached to it.

### ***Appendix III***

#### **TABULATIONS OF DETAILED DATA**

TABLE 1  
FINE AGGREGATE FOR BITUMINOUS CONCRETE MIXTURES

Agency	Kinds of Material Used									Angularity of particles in Specification	
	Natural Sand	Stone Screenings	Cr Gravel Screenings	Stone Sand	Mine Tailings	Chat	Slag Screenings	Volcanic Cinders	Nat Sand Screenings	Specs	Specification
1 Ala.	x								x	No	2/
2 Ariz.	x			x				x		No	
3 Ark.	x	x								No	
4 Calif.	x	x		x						No	
5 Colo.	x									No	
6 Conn.	x								x	Yes	100% rough & angular Stone screenings
7 Del.		x								Yes	
8 D. of C.	x	x								No	
9 Fla.	x	x					x		x	No	
10 Ga.	x	x								No	
11 Idaho	x			x						No	
12 Ill.	x	x		x		x				No	
13 Ind.	x		x	x			x		x	No	
14 Iowa	x	x								No	
15 Kans.	x	x			x					No	
16 Ky.	x			x			x			No	30-50% angular
17 La.	x	x								No	
18 Me.	x	x								No	
19 Ma.	x	x		x			x			No	
20 Mass.	x								x	Yes	50% max screenings
21 Mich.	x			x						No	
22 Minn.	x									No	
23 Miss.	x	x					x		x	No	
24 Mo.	x				x	x				No	
25 Mont.	x	x								Yes	50-75% Angular
26 Nebr.	x									No	
27 Nev.	x			x						No	
28 N.H.	x	x								Yes	50% natural sand
29 N.J.	x	x								No	
30 N.M.	x	x	x						x	No	
31 N.Y.	x	x		x						No	
32 N.C.	x	x							x	No	
33 N.Dak.	x									No	
34 Ohio	x			x			x			No	
35 Okla.	x	x		x		x				No	
36 Oreg.	x	x	x							No	Moderately sharp
37 Pa.	x	x	x				x			No	
38 R.I.	x									No	
39 S.C.	x	x								No	
40 S.Dak.	x									No	
41 Tenn.	x	x	x				x			No	
42 Tex.	x	x								No	
43 Utah	x	x	x							No	
44 Vt.	x								x	No	
45 Va.	x	x							x	No	
46 Wash.	x	x	x							No	
47 W. Va.	x	x		x			x			No	
48 Wisc.	x	x								No	
49 Wyo.	x									No	
50 Ontario	x	x	x						x	No	

1/ Stone for sand and screenings, 10 cycles of testing  $Mg SO_4$ , loss not to exceed 7%,  $Mg SO_4$ , loss

2/ Minimum of 30 percent of total aggregate must be coarse, sharp concrete sand.

Note: Whenever the phrase "Not specified" is used in this and following tables, it means that the r

TABLE 1 (continued)

Limitation of Deleterious Materials											Soundness Requirements	
Organic Vegetable Roots, Etc	Clay Loom	Clay Lumps	Finer than No 200 or Decanted	Soft	Coal Lignite	Shale	Cemented	Other	Undif- feren- tiated	Total Allowable	Method of Test	Specified Maximum Loss
(allowable percent shown when specified)											(percent)	
		0.5			0.5	1		1.0 (mica, alkali)		3	Na <sub>2</sub> SO <sub>4</sub>	10
			12		(PT 5-)			0.5 (cinders clinkers)	1	12	Not specified	
		1				x				5	Not specified	
					No specific requirement						Not specified	
					No specific requirement						L. A. wear on parent mtrl	- 45%
					No specific requirement						Not specified	
					No specific requirement						Not specified	
0	0								0	None	Na <sub>2</sub> SO <sub>4</sub>	12
									0	None	Not specified	
		6								6	Not specified	
Not specified for F A separately (LL 35-, PI 6-)											Not specified	
		1			1		1			3	Na <sub>2</sub> SO <sub>4</sub>	10
		0.2			x	2				5	Na <sub>2</sub> SO <sub>4</sub>	10
			3			2				5	Freeze-Thaw on Parent Material	(16 cycles 25)
1	1			5						5	Special Freeze-Thaw	Loss Ratio 0.85-
		1	1		1					3	Na <sub>2</sub> SO <sub>4</sub>	10
0	0	0							0	None	Not specified	
										None	Not specified	
		0	1		1				3	5	Na <sub>2</sub> SO <sub>4</sub>	15
		0							0	None	Not specified	
x			5								Not specified	
		0				0				None	Not specified	
		3	(AASHTO M-79 used with slag and stone screenings)							3	Not specified	
					3					3	Not specified	
0	0	0							0	None	Not specified	
1	x				x	x		x (alkali)			Na <sub>2</sub> SO <sub>4</sub>	15
	x								x	3	Not specified	
Quantity of deleterious material must be negligible											Not specified	
0	0				0			0 (mica, salt)	0	None	Not specified	
0	0									None	Mg SO <sub>4</sub>	12
		(adobe)										
0	0	0							0	8	1/	1/
		15 (of minus No. 10 fraction)				12 (of total mixture)					Not specified	
0		0								None	Na <sub>2</sub> SO <sub>4</sub>	10
0.1		1								1.1	Not specified	
	x								x	2	Not specified	
									0	None	Na <sub>2</sub> SO <sub>4</sub>	10
	0								0	None	Mg SO <sub>4</sub>	-
											Not specified	
0	0									None	L. A. wear - 45 max. Swell T-101 - 13 max.	
	0.5		3	3		0.5				5	Na <sub>2</sub> SO <sub>4</sub> on Stone Sand	12
No specific requirement (PI 6-) x Free of excessive quantity x (disintegrating)											Not specified	
0		0.25	1			1		1 (mica)	0	None	Na <sub>2</sub> SO <sub>4</sub>	8
										1.25	Freeze-Thaw	15 cycles - 8
											Mg SO <sub>4</sub>	5 cycles - 8
No specific requirement											Not specified	
		x	3		x						Na <sub>2</sub> SO <sub>4</sub>	10
0	0	0							0	None	Not specified	
0										None	Not specified	
No specific requirement											Mg SO <sub>4</sub>	
											16	

not to exceed 12%. Natural sand, 10 cycles of testing: Na<sub>2</sub> SO<sub>4</sub>, loss not to exceed 8%, Mg SO<sub>4</sub>, loss not to exceed 22%.

porting agency does not have a specification requirement covering the item listed





TABLE 1 (continued)

or Fine Aggregate											1954 Practice					
Surface Course Material											Agency					
No. 4	No. 8	No. 10	No. 16	No. 20	No. 30	No. 40	No. 50	No. 80	No. 100	No. 200						
except when stated otherwise)																
Not specified											Ala. 1					
Not specified											Ariz. 2					
Not specified											Ark. 3					
Not specified											Calif. 4					
68-84											Colo. 5					
95	100										8					
Not specified											Del. 7					
95-100	45-80			10-30			2-10				D. of C. 8					
98-100	0-15	Passing and retained			30-60			15-40			0-15	Fla. 9				
Not specified											Ga. 10					
95-100	0-15	Passing and retained			20-60			15-35			0-5	Idaho 11				
15-50											5					
0-10	15-35	Passing and retained			5-35			1-10			0-5	Ill. 12				
25-65											5					
Not specified											Ind. 13					
Not specified											Iowa 14					
Not specified											Kans. 15					
90-100	75-90	40-80			5-35			0-15			0-10	Ky. 16				
Not specified											La. 17					
Passing and retained											7-14					
15-40											14					
100											75-90					
35-65											15-30					
5-12											Mass. 20					
100-98	0-5	Passing and retained			30-60			15-35			0-5	Mich. 21				
5-35											5					
98-100	8-25	Passing and retained			22-65			7-40			0-8	Minn. 22				
15-50											8					
Not specified											Miss. 23					
Not specified											Mo. 24					
98-100	0-15	Passing and retained			30-60			15-40			0-5	Mont. 25				
15-50											5					
5-40	45-70			60-85			90-			95-		Nebr. 26				
100	95-100			55-75			25-50			0-12		Nev. 27				
Not specified (except No. 200)											0-15	N.H. 28				
Passing and retained											0-5	N.J. 29				
6-30											15-42					
Not specified											20-40					
Not specified											12-35					
Not specified											5	N.M. 30				
Not specified											N.Y. 31					
Not specified											N.C. 32					
Not specified											N.Dak. 33					
90-100	65-100	40-85			20-60			7-40			0-15	0-7	Ohio 34			
Not specified											Okla. 35					
% retained											90-100	Oreg. 36				
0	25-40											Pa. 37				
100											85-98	65-90	40-75	5-30	0-6	R.I. 38
100-0-10	15-40			30-60			5-35			5-20			0-5	S.C. 39		
Not specified											S.Dak. 40					
Not specified											Tenn. 41					
Not specified											Tex. 42					
Not specified											Utah 43					
Not specified											Vt. 44					
Not specified											Va. 45					
Passing and retained											5-16	Wash. 46				
30-55											20-50					
95-100	80-95	50-85			5-25			0-7				W. Va. 47				
Not specified											Wisc. 48					
Not specified											Wyo. 49					
95-100	80-100	#14			35-70			15-40			5-15	0-5	Ontario 50			
55-90																

TABLE 2  
COARSE AGGREGATE FOR BITUMINOUS CONCRETE MIXTURES

Agency	Kinds of Material Used								Uncrushed Gravel Particles		Wear Requirements		Soundness Method 1/ of Test
	Crushed Gravel	Crushed Stone	Gravel	Crushed Slag	Vol- canic Cinders	Mine Chats	Crushed Boulders	Lava			Test Method	Allowable Percent Loss	
									Permitted	Percent (of CA)			
1 Ala.	x	x		x					No	-	L.A.	48	Na <sub>2</sub> SO <sub>4</sub>
2 Ariz.	x	x	x		x				Yes	-	L.A.	40	Not
3 Ark.	x	x							No	-	Deval	6 stone 15 gravel	Na <sub>2</sub> SO <sub>4</sub>
4 Calif.	x	x	x						Yes	-	L.A.	50	Not
5 Colo.	x	x		x					Yes	50	L.A.	45	Not
6 Conn.	x	x							Yes	50	L.A.	40	-
7 Del.		x							No	-	L.A.	40	Not
8 D. of C.		x		x					No	-	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
9 Fla.		x		x					No	-	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
10 Ga.		x		x					No	-	L.A.	60	-
11 Idaho	x	x	x						Yes	-	L.A.	40	Not
12 Ill.	x	x		x			x		No	-	L.A.	35	Na <sub>2</sub> SO <sub>4</sub>
13 Ind.	x	x		x					No	-	L.A.	40 to 45	Freeze-Thaw
14 Iowa	x	x							Yes	40 (Total agg.)	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
15 Kans.	x	x				x			Yes	50 (Total agg.)	L.A.	45	Freeze-Thaw
16 Ky.	x	x	x	x					Rarely	-	L.A.	35	Na <sub>2</sub> SO <sub>4</sub>
17 La.	x	x	x						Yes	40 (Plus No. 10)	Deval	7 stone 15 gravel	Not
18 Me.	x	x							Yes	50	L.A.	40	-
19 Md.		x		x					Yes	30	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
20 Mass.		x							No	-	L.A.	30 to 35	Not
21 Mich.		x					x		No	-	L.A.	32	Mg SO <sub>4</sub>
22 Minn.	x	x							No	-	L.A.	35	-
23 Miss.	x	x	x	x					Yes	-	L.A.	40 stone & slag 35 gravel	Na <sub>2</sub> SO <sub>4</sub>
24 Mo.	x	x	x			x			Yes	-	Deval	6+ (Fr. coef.)	Not
25 Mont.	x	x							Yes	25	L.A.	40	Not
26 Nebr.	x	x	x						Yes	-	L.A.	40	Freeze-Thaw
27 Nev.	x	x							No	-	L.A.	37	-
28 N.H.	x	x							Yes	50	L.A.	40	Not
29 N.J.	x	x	x						Yes	-	Deval	3.5	Not
30 N.M.	x	x						x	Yes	50	L.A.	50	Mg SO <sub>4</sub>
31 N.Y.		x		x					No	-	Deval	5.7	Na <sub>2</sub> SO <sub>4</sub>
32 N.C.		x		x					No	-	L.A.	55	Not
33 N.Dak.	x		x						Yes	-	No specified reqm't		Not
34 Ohio	x	x		x					Yes	60	No specified reqm't		Na <sub>2</sub> SO <sub>4</sub>
35 Okla.	x	x	x						Yes	-	L.A.	40	Not
36 Oreg.	x	x			x				Yes	40	L.A.	30	Not
37 Pa.	x	x		x					No	-	L.A.	10(100 rev.) 35(500 rev.)	Na <sub>2</sub> SO <sub>4</sub>
38 R.I.	x	x	x						Yes	-	L.A.	40	Mg SO <sub>4</sub>
39 S.C.	x	x	x	x					Yes	25	L.A.	60	Not
40 S.Dak.	x	x							No	-	L.A.	45	Not
41 Tenn.	x	x		x					No	-	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
42 Tex.	x	x	x						Yes	-	L.A.	40	Not
43 Utah	x	x							Yes	30	L.A.	40	Na <sub>2</sub> SO <sub>4</sub>
44 Vt.	x	x							No	-	Deval	5 stone 16 gravel	Na <sub>2</sub> SO <sub>4</sub>
45 Va.		x		x					No	-	L.A.	5 (100 rev.) 3 (500 rev.)	Mg SO <sub>4</sub>
46 Wash.	x	x							Yes	25	L.A.	30	Freeze-Thaw
47 W.Va.	x	x		x					No	-	L.A.	40	Not
48 Wisc.	x	x							Yes	50-	L.A.	50	Na <sub>2</sub> SO <sub>4</sub>
49 Wyo.	x	x							No	-	L.A.	50	Not
50 Ontario	x	x							Yes	40	L.A.	35	Mg SO <sub>4</sub>

1/ Where the Na<sub>2</sub> SO<sub>4</sub> (sodium sulfate) or Mg SO<sub>4</sub> (magnesium sulfate) tests are indicated, a 5-cycle exposure is used except where

TABLE 2 (continued)

Requirements Specified 1/ Maximum Loss (percent)	Limitation of Deleterious Materials							
	Organic, Vegetable, Roots, Etc.	Clay Loam	Clay Lumps	Finer Than No.200 or Decanted	Soft Lignite	Coal	Shale	Other
	(allowable percent shown when specified)							
10 specified			0.25	0.5	2	0.25		
12			1		x	No specific requirement	x	
specified						No specific requirement		
specified						No specific requirement		
- specified						No specific requirement		
12						No specific requirement		
12	0.03	0(dirt)	0.05	1.25	10	1		0.5(cinders) 1.0(shells)
15 specified		1				No specific requirement		
15(5 cycles)			0.5	2.5	5	1		
15(50 cycles)								
20			0.2	1	4		2	1.0(ocher) 1.0(shells)
10(16 cycles)			0.5	3			3	
0.85 Loss Ratio			2		5	0.5	0.5	
15 specified		1					2	2
-								0
15 specified			1		5	1	1	3
12					3			15
-							0(in cr. stone) 3(iron oxide)(in cr.gr.)	0(cr.gravel)
12		x				x	x	x(cinders)
specified	0.25		1.0(& shale)		8		x	
specified	0	0	0					
0.90 Loss Ratio	1	x		x	x		x	x(alkali)
-								
specified								Quantity of deleterious material must be negligible
specified					2			3
12	0	0(adobe)						
7(10 cycles)								No specific requirement
12(10 cycles)								
specified	0	0					12(of total aggregate)	
specified		0					2.5	
12	0.1		0.25	1	3	1		
specified		0(dirt)	1	3	5			0
specified			0.25	2	2	1	1	4(glassy in slag) 2(iron in slag)
10								
12		0(dust)						0
specified	0			0				0
specified	0	0						
12			0.25	1.25	5		1	
specified				2(PT +6) 4(PT -6)				
12							No specific requirement	
8				x			x	x(schist)
8( 5 cycles) 8(15 cycles)			0.25	0.5				
specified	0							
12			0.25			1	1	
specified	0	0	0					
specified			0					0
12								No specific requirement

noted.



TABLE 2 (continued)

1954 Practice

Specified Gradation Limits for Coarse Aggregate														Agency		
Surface Course Material																
No. 4	No. 8	No. 10	1"	3/4"	5/8"	1/2"	3/8"	No. 4	No. 8	No. 10	No. 16	No. 20	No. 30	No. 200		
by weight passing each sieve, except when stated otherwise)																
Not specified														1 Ala.		
Not specified														2 Ariz.		
Not specified														3 Ark.		
Not specified														4 Calif.		
Not specified														5 Colo.		
Not specified														6 Conn.		
Not specified														7 Del.		
0-10	0-5	0-3	100	90-100	85-100	45-85	25-40	0-10	0-5	0-8				8 D of C.		
0-10	0-5										100	90-100	20-55		5-30	0-10
0-15											100	95-100	20-50		Not specified	0-5
Not specified														9 Fla.		
Not specified														10 Ga.		
Not specified														11 Idaho		
Not specified														12 Ill.		
95-100	98-100	Percent Retained												13 Ind.		
		0 5-25 70-95 95-100												14 Iowa		
Not specified														15 Kans.		
Not specified														16 Ky.		
5-25	0-5	100 80-100 10-30 0-5 0-3												17 La.		
Not specified														18 Mo.		
Not specified														19 Md.		
5-15	0	0-10	100	80-100	30-50	0								20 Mass.		
	0-10						100	90-100	10-25	0-10						
							100	95-100	40-70	0-25	0-5					
Not specified														21 Mich.		
Not specified														22 Minn.		
Not specified														23 Miss.		
Not specified														24 Mo.		
Not specified														25 Mont.		
Not specified														26 Nebr.		
0-5		0 0-10	95-100	35-55	30-65	80-100	0-5	90-100	95-100					27 Nev.		
			100	60-85	15-35	0-5	0-5	0-2						28 N.H.		
Not specified														29 N.J.		
Not specified														30 N.M.		
Not specified														31 N.Y.		
Not specified														32 N.C.		
Not specified														33 N.Dak.		
100	95-100	65-90	35-65	0-15										34 Ohio		
Not specified														35 Okla.		
% Retained														36 Oreg.		
0-10	0-5	0	25-40	90-100	10-30	0-10								37 Pa.		
100 75-100 0-15 0-5														38 R.I.		
Not specified														39 S.C.		
Not specified														40 S.Dak.		
Not specified														41 Tenn.		
Not specified														42 Tex.		
Not specified														43 Utah		
Not specified														44 Vt.		
Not specified														45 Va.		
Not specified														46 Wash.		
0-5		100	85-100	20-40	0-10									47 W.Va.		
Not specified														48 Wisc.		
Not specified														49 Wyo.		
0-10		100	83-100	50-70	0-10									50 Ontario		

TABLE 3  
MINERAL FILLER FOR BITUMINOUS CONCRETE MIXTURES

Agency	Kinds of Material						Remarks	Specified Gradation Limits						
	Lime-Stone Dust	Port-land Cement	Min-eral Dust	Stone Dust	Inert Mineral Matter	Other Types		No.10	No.30	No.40	No.50	No.80	No.100	
								(percent by weight finer than each size except when stated otherwise)						
1 Ala.	x	x			x		Nonplastic, nonhydrophilic	100				95-100		
2 Ariz.									Not specified					
3 Ark.	x	x							100					
4 Calif.	x	x	x			Hydrated lime			100					
5 Colo.	x	x				Hydrated lime			100					
6 Conn.	x	x		x					100				95-100	
7 Del.	No mineral filler required						Special approval for inert mineral matter	No mineral filler required						
8 D. of C.	x	x						100				95-100		
9 Fla.	x	x			x			100				95-100		
10 Ga.	x	x									100	90-		
11 Idaho							Other types on approval							
12 Ill.	x							100					85-	
13 Ind.	x	x		x	x	Fly ash						(percent retained)		
14 Iowa	x	x						0				0-5		
15 Kans.	x	x				Chat sludge		100				95-100		
16 Ky.	x	x			x			100				95-100		
17 La.	x	x				Shell dust		100				95-100		
18 Me.					x		Stone float or collector dust on special permission	100					85-	
19 Md.	x	x	x					100						
20 Mass.	x	x										100		
21 Mich.	x	x				Fly ash						100		
22 Minn.	x	x			x				No. 20					
23 Miss.	x	x			x			100	95-100			80-100		
24 Mo.	x	x	x	x	x			100				95-100		
25 Mont.		x		x				100					85-	
26 Nebr.	x					Natural soil						(percent retained)		
27 Nev.	x	x				Basalt rock dust	Any approved material	100				95-100		
28 N.H.	x	x		x				100						
29 N.J.	x		x		x	Fly ash							95-	
30 N.M.						Fly ash						Not specified		
31 N.Y.	x	x				Diatomaceous earth		100					85-100	
32 N.C.	x	x	x					100				95-100		
33 N.Dak.						Natural soil	No mineral filler required							
34 Ohio	No mineral filler required													
35 Okla.		x		x		Volcanic ash								
36 Oreg.		x	x					100				95-100		
37 Pa.		x		x								100		
38 R.I.	x	x	x					100				90-100		
39 S.C.	x	x	x					100						
40 S.Dak.				x		Silt			100			95-100		
41 Tenn.	x	x						100		100				
42 Tex.		x	x	x	x	Shell dust		100						
43 Utah	x	x	x					100				95-100		
44 Vt.	x					Talc dust	Any approved material			100				
45 Va.	x	x			x			100				95-100		
46 Wash.	x	x				Cottrell flour Basalt rock dust		100						
47 W.Va.	x	x			x		Any approved material Minus No.4 sieve fraction		100				90-	
48 Wisc.	x	x	x					100				85-100		
49 Wyo.									Not specified					
50 Ontario	x							100						

TABLE 3 (continued)

1954 Practice

No.200 size,	Remarks	Agency
65-100	AASHO M17-42 gradation	1 Ala.
75-100		2 Ariz.
75-100	Gradation continued 0-25 percent finer than .005 mm.	3 Ark.
75-100	Gradation continued 25-100 percent passing No. 270 sieve	4 Calif.
75-100		5 Colo.
		6 Conn.
65-100	AASHO M17-42 gradation	7 Del.
65-100	AASHO M17-42 gradation	8 D.of C.
65-100		9 Fla.
65-100	PI 6-, LL 25-; Dust Ratio less than 65 percent	10 Ga.
65-100		11 Idaho
0-35	AASHO M17-42 gradation	12 Ill.
65-100	AASHO M17-42 gradation	13 Ind.
100	Mineral filler (minus No.200) present in crushed aggregates of total mix acceptable, mineral filler in uncrushed aggregates of total mix acceptable provided this portion of filler does not exceed 50% of total.	14 Iowa
65-100	AASHO M17-42 gradation	15 Kans.
65-100	Gradation continued 60-100 percent finer than .05 mm, 30-60 percent finer than .020 mm, 10-25 percent finer than .005 mm; 2-15 percent finer than .001 mm.	16 Ky.
65-100		17 La.
65-100		18 Mo.
65-100		19 Md.
65-100		20 Mass.
75-100	Fly ash - Free carbon 7-12 percent Minus No. 200 material - 15 to 60 percent less than .01 mm. size.	21 Mich.
60-100		22 Minn.
65-100	AASHO M17-42 gradation	23 Miss.
75-100	Gradation continued, 30-100 percent passing No. 325 sieve.	24 Mo.
65-100		25 Mont.
0-20		26 Nebr.
65-100	AASHO M17-42 gradation	27 Nev.
65-100		28 N.H.
65-100		29 N.J.
65-100	PI 6-, LL 25-	30 N.M.
		31 N.Y.
65-100	AASHO M17-42 gradation	32 N.C.
40-100	Gradation continued 0-20 percent finer than .005 mm.	33 N.Dak.
		34 Ohio
65-100	AASHO M17-42 gradation	35 Okla.
67-100		36 Oreg.
75-100		37 Pa.
70-100		38 R.I.
60-100	PI 12-; WAP 25-; Lineal Shrinkage 4-	39 S.C.
65-100	AASHO M17-42 gradation	40 S.Dak.
65-100		41 Tenn.
65-100	AASHO M17-42 gradation	42 Tex.
65-100		43 Utah
65-100	AASHO M17-42 gradation	44 Vt.
75-100	Gradation continued 50-100 percent finer than .025 mm, 0-35 percent finer than .005 mm. PI 2-.	45 Va.
65-100		46 Wash.
65-100		47 W.Va.
		48 Wisc.
		49 Wyo.
30-100	Mineral litter not generally used because of low void content in mineral aggregate.	50 Ontario



TABLE 4  
ASPHALT CEMENT FOR BITUMINOUS CONCRETE MIXTURES

Agency	Penetration	Specification Requirements							Spot Test ST'd Naphtha	1/ - Negative Spot Reg'd.			Specific Gravity	Other Specific Requirements
		Bitumen Soluble in		1/ Ductility	1/ 2 Flash Point	1/ Loss on Heating	Penetration Residue 1/ Before Heating	Naphtha		Xylene	Heptane			
		Carbon Disulfide	Carbon Tetrachloride											
1 Ala	60-70 85-100 100-120	99 5+		100+	450+	0 5+	70+	Neg				N S 3/	Ductility at 39 2°F not less	
2 Ariz	150-200	99 5+		100+	347+	1 0-	65+				35	N S		
3 Ark	60-70 70-85		99 5+	100+	450+	1 0-	70+	Neg				N S		
4 Calif.	85-100	99 5+		100+	425+	2 0-	80+				35	N S.		
5 Colo	120-150	99 5+		100+	425+	2 0-	70+			10		N S		
6 Conn	85-100	99 5+		100+	347+	1 0-	60+			Not specified		N S		
7 Del	70-85	99 5+		Penetration value + 100+	347+	1 0-	75+	Neg				N S		
8 D of C.	85-100	99 5+		100+	347+	1 0-	65+	Neg		Not specified		N S		
9 Fla	85-100	99 5+	99 0+	100+	347+	1 0-	65+					N S		
10 Ga	85-100		99 5+	100+	400+	1 0-	70+	Neg				1 00+ N S		
11 Idaho	121-150	99 5+	99 0+	100+	400+	1 0-	65+				35	N S		
12 Ill.	70-85	99 5+		100+	500+	1 0-	70+	Neg				N S		
13 Ind	85-100	99 5+		100+	450+	1 0-	70+	Neg.				N S	Other penetration grades per	
14 Iowa	85-100	99 5+	99 0+	100+	347+	1 0-	65+	Neg				N S	Softening point 130°F -125°F	
15 Kans	85-100		99 5+	100+	347+	1 0	75+	Neg				N S	Softening point 104°F -140°F	
16 Ky	85-100	99 5+	99 0+	100+	347+	1 0-	75+			Not specified		N S		
17 La	85-100	99 5+		100+	347+	1 0-	65+	Neg		Not specified		N S		
18 Me	85-100	99 5+		100+	450+	1 0-	50+				35	1.00+ N S.		
19 Mi	85-100	99 0+		100+	347+	1 0-	65+					N S		
20 Mass	85-100	99 5+		100+	347+	1 0-	65+			Not specified		N S	For recovered asphalt (ASTM Penet 50+ pct of original)	
21 Mich	60-70 85-100		99 5+	130+ 100+	347+ 347+	1 0- 1 0-	75+ 65+	Neg				1 01+ 1 00+	For recovered asphalt (ASTM Penet 50+ pct of original)	
22 Minn	70-85 85-100		99 0+	100+	450+	1 0-	70+	Neg				N S	pet of original 40-7) pen	
23 Miss	85-100	99 5+		100+	400+	1 0-	60+	Neg				1 01- 10 02	Heat to 347°F without foam	
24 Mo	70-85	99 5+		100+	450+	1 0-	60+	Neg				N S	Penetrations of 60-70 and 9	
25 Mont	70-85 85-100	99 5+		100+	347+	1 0-	70+					N S	Heat to 347°F without foam	
26 Nebr	85-100	99 5+	99 5+	100+	347+	1 0-	80+			10		N S		
27 Nev.	85-100 100-120 120-150	99 5+		100+	450+	3 0-	70+			Not specified		N S		
28 N H	85-100 100-120		99 0+	100+	450+	1 0-	75+			Not specified		1 00- 1 00-	1 Heat to 347°F without foam	
29 N J	60-70 70-85	99 5+	99 0+	100+	450+	1 0-	70+			Not specified		N S	2 Penetration 85-100 used	
30 N H	85-100	99 5+	99 0+	100+	347+	1 0-	75+			Not specified		N S	Heat to 347°F without foam	
31 N Y	85-120	99 5+		60+	347+	1 0-	60+			Not specified		1 00- 1 01	ditto	
32 N C	85-100	99 5+		100+	347+	1 0-	60+	Neg				N S	1 Heat to 347°F without foam	
33 N Dak	120-150 150-200	99 5+	99 0+	100+	347+	1 0-	65+	Neg				N S	2 Use grade with penetration	
34 Ohio	70-80	99 5+		100+	347+	1 0-	70+					N S	2 For recovered asphalt (A	
35 Okla	85-100	99 5+		100+	450+	0 2-	65+	Neg				N S	Penetration 65+ percent	
36 Oreg	86-100	99 5+		100+	400+	1 0-	65+	Neg				N S	Flash point 400°F	
37 Pa	70-80 85-100	99 5+		100+	350+	1 0-	75+	Neg				N S	Loss on heating 1 0- per	
38 R I	61-70	99 0+		90+ 70+	350+ 347+	1 0- 1 0-	65+ 75+	Neg				N S	Penet, residue/before he	
39 S C	60-70 85-100	99 0+		Penetration value + 100+	347+	1 0-	75+			Not specified		N S	Ductility 100+ cm	
40 S Dak	100-120 120-150		99 0+	100+	347+	2 0-	60+			15		N S	Bitumen Soluble in Carbon	
41 Tenn	85-100	99 5+		100+	347+	1 0-	65+	Neg				N S	Naphtha xylene, negative	
42 Tex	85-100	99 5+	99 5+	100+	450+	0 75+	50+	Neg				N S	Heat to 351°F without foam	
43 Utah	85-100	99 5+	99 0+	100+	347+	1 0-	65+					N S	30+ percent	
44 Vt	85-100	99 5+		100+	347+	1 0-	75+	Neg		Not specified		30	1 Use grade with penetrati	
45 Va	85-100	99 5+		100+	350+	1 0-	75+					N S	2 For recovered asphalt (A	
46 Wash	86-100	99 0+	99 65+	100+	450+	1 0-	70+	Neg				N S	Penet 65+ pct of orig	
47 W Va	85-100	99 0+		100+	450+	1 0-	75+					N S	Ash -1.0 percent	
48 Wisc	70-85	99 5+	99 5+	100+	450+	1 0-	70+	Neg				N S	Heat to 347°F without foam	
49 Wyo	85-100	99 5+		100+	450+	1 0-	70+			15		N S	Heat to 350°F without foam	
50 Ontario	121-150 85-100	99 5+		60+ 100+	425+ 450+	2 0- 1 0-	70+			Not specified		N S	Heat to 350°F without foam	

1/ Conditions of test are AASHTO standard  
2/ Cleveland Open Cup (AASHTO T 48-46)  
3/ Not specified



TABLE 5

MINERAL AGGREGATE GRADATION REQUIREMENTS AND BITUMEN CONTENT  
OF BITUMINOUS CONCRETE BINDER-COURSE MIXTURES

Agency	Method of Specifying Sieve-Size Limits	Basis of Per- centage Limits	Gradation Specifications Standard Sieve Size or Num									
			2"	1-1/2"	1-1/4"	1"	3/4"	5/8"	1/2"	3/8"	1/4"	No. 4
			(figures are per cent)									
1 Ala.	Percent passing	Total aggregate					100	75-100	55-95	47-87		35-67
2 Ariz.							Gradation limits specified in construction special prov					
3 Ark.	Percent retained	Total aggregate					0	5-20	20-40			45-60
4 Calif.	Percent passing	ditto					100	95-100		60-75		40-55
	ditto	"					100	95-100		65-80		45-60
5 Colo.	"	"					100	90-100		60-80		32-43
6 Conn.	"	"					90-100		45-75			
7 Del.	"	"					100	90-100	50-80	40-65		25-45
8 D. of C.	"	"					100	90-100		40-80		20-40
9 Fla.	Pct. pass & ret 1/	"					k--		65-85			
10 Ga.	Percent passing	"					100	75-100		40-75		
11 Idaho	ditto	"					100				48-58	
12 Ill.	Pct pass. & ret.	Total mixture	95-100	passing		*	25-	*		10-60		20-45
13 Ind.	ditto	ditto					k	5-50	*			
14 Iowa	Percent passing	Total aggregate					100	98-100		67-87		47-60
15 Kans.	Percent retained	ditto					0	0-5		15-45		35-50
16 Ky.	Percent passing	"					100	90-100		55-80		35-60
17 La.	ditto	"					100	90-100				25-40
18 Me.	"	"					100	93-100	82-95	71-88	61-77	40-51
19 Md.	"	"					0		5/30-50 6/		15-30	*
20 Mass.	Pct pass & ret	Total mixture	100	passing		*				60-80		
21 Mich.	ditto	ditto					100	95-100				40-60
22 Minn.	Percent passing	Total aggregate					100	85-100	68-90	62-85		47-60
23 Miss.	ditto	ditto								10-40		*
24 Mo.	Pct pass. & ret	Total mixture	100	pass. *	0-5		*0-20	*	10-40			25-70
25 Mont.	Percent passing	Total aggregate					0	0-4		5-30		35-50
26 Nebr.	Percent retained	ditto						0				
	ditto	"						95-100		58-70		28-54
27 Nev.	Percent passing	"						100	60-90	50-80		30-50
28 N. H.	ditto	"								0-20	*	
29 N. J.	Pct pass & ret	Total mixture	3/	k	0-35	*		35-70				30-60
30 N. M.	Percent passing	Total aggregate					100		65-100			30-60
31 N. Y.	Pct pass & ret	Total mixture					k0-5	*	35-60	*	20-40	5-10
32 N. C.	ditto	ditto	100	passing			*	0-10	*	15-40	*	35-60
33 N. Dak.	Percent passing	Total aggregate					100					50-83
34 Ohio									Binder course not			
35 Okla.	ditto	ditto	100				90-100		65-80			40-50
36 Oreg.	Pct pass & ret.	Total mixture	100	passing		*				40-52		*
37 Pa.	Percent passing	Total aggregate					90-100		40-75			20-40
38 R. I.	ditto	Total mixture			100							
39 S. C.	"	Total aggregate					100	90-100	97-100	60-95		30-60
40 S. Dak.	"	ditto						69-85	75-90		50-75	43-50
41 Tenn.	"	"					100	55-80				25-40
42 Tex.	Pct. pass & ret.	Total mixture	3/0-3*	15-40		*		15-40	*	10-25	*	
43 Utah	Percent passing	Total aggregate					95-100	75-100	60-90		35-65	25-50
44 Vt.	ditto	ditto						100		65-90		22-60
45 Va.	"	"					100	95-100		60-80		40-60
46 Wash.	Pct pass & ret.	" 8/							k 0-10	*	25-45	*
47 W. Va.	Percent passing	"	100	95-100				60-75		30-50		20-40
48 Wisc.	ditto	"					95-100		65-90	55-80		40-60
49 Wyo.	"	"						100		60-85		45-60
50 Ontario	"	"					2/ 100	75-94	65-88	54-80	40-68	33-57

1/ Percent of material passing one sieve and retained on the next finer sieve.

2/ Percent of total aggregate.

3/ Round sieve-openings, 1/4 inch size and larger.

4/ Passing No. 4, retained No 6 sieve, 0-5 percent, passing No 6, retained No. 8, 0-5 percent

5/ 7/8-inch sieve

6/ Not more than 1/5 of the 7/8 to 1/2-inch fraction in the bottom course shall be retained on a 3/4-inch sieve.

7/ Percent passing

8/ Percent limitations for material finer than No. 10 based on total fraction passing No. 10. Of total aggregate, 2/

9/ No 14 sieve.

TABLE 5 (continued)

1954 Practice

General Aggregate								Specified	Remarks	Agency
Square Openings								Bitumen Content		
No. 8	No. 10	No. 16	No. 20	No. 30	No. 40	No. 50	No. 80	No. 100	No. 200	
(by weight)								of Mixture		
								(pct. by wt.)		
24-50				12-30			4-15		2-8	5-8 2/
Sources for designated aggregate sources.										
60-75				75-90					95-100	3.7 - 7.7
			12-22						3-6	3.0 - 7.0 2/ Heavy traffic
			15-25						3-7	3.0 - 7.0 2/ Medium traffic
			19-27						1-5	4.5 - 5.5
15-35									5-10	3.5 - 6.0
20-35		15-25		10-20			8-15		5-10	4.0 - 6.0
15-35									0-5	4.0 - 7.0
*15-35										4.0 - 7.0
					5-20			0-10	0-5	4.5 - 7.0
30-40									3-9	Not specified
*3-12	*		20-35				2-10	*0-4	*0-3	4.0 - 7.0
		5-20					6+		3-10	6.25
		19-34			13-26		90+		93-98	5.0 - 7.0 2/
		85+				0-15			0-5	4.0 - 7.0
25-40				15-30			8-18		2-6	4.0 - 6.0
18-38		15-35		8-25						4.0 - 6.5
22-36		13-25		8-18			5-13		2-8	4.0 - 6.5
*2-8	*	*4-10			4-10	*	2-6	*1-4		4.5 - 5.5
				14-36						4.0 - 6.0
25-40									0-5	4.2 - 5.0
40-58				24-38		10-22			6-10	4.7 - 6.2
*15-60		4-18			3-20	*	2-15	*2-8		3.5 - 6.0
55-75									0-5	4.0 - 6.5
55-75					78-88	85-93	90-95		89-95	4.5 - 6.0 2/ Heavy traffic
25-38				15-25	77-87	8-16			2-6	4.5 - 6.0 2/ Medium traffic
22-42		14-32		10-27						3.0 - 7.0
*0-10	*			2-8	*	2-12	*0-5			4.0 - 6.5
20-45									3-12	4.0 - 5.5
*4-20	*									4.0 - 5.5
25-60				15-40				*0-5		4.0 - 6.5
		15-42		10-28		5-17		0-8		3.0 - 7.0
30-45				20-30		10-20		1-7		4.0 - 6.5
*12-20					3-9	*3-7	*3-7			5.0 - 7.0
10-25		5-20			2-15		1-10	0-5		4.3 - 7.0
15-35										4.0 - 6.0
15-30										4.5 - 7.0
35-55				20-30				6-10		5.0 - 7.0
		22-30				2-8				4.5 - 5.5
						5-15				3.5 - 6.0
*0-15	*			3-15	*	3-15	*4-10			3.0 - 6.0
20-40				10-30		5-20	3-8			4.5 - 6.0
17-55				13-48		8-23	4-7			5.0 - 7.0
20-40						3-10				4.5 - 8.0
*20-55	*			15-45	*	10-35	*4-15			4.0 - 7.0
10-25				3-10						3.0 - 6.0
25-50				10-30					3-12	3.5 - 6.0
25-45									3-10	4.5 - 6.5
2/ 12-45		6-35		3-20		1-8		0-5		4.5 - 6.0 2/

Percent permitted to pass no. 10 sieve.

TABLE 6

**MINERAL AGGREGATE GRADATION REQUIREMENTS AND BITUMEN CONTENT  
OF BITUMINOUS CONCRETE SURFACE-COURSE MIXTURES**

Agency	Method of Specifying Sieve-Size Limits	Basis of Per- centage Limits	Gradation Specifications - Mineral Aggregate											
			Standard Sieve Size or Number - Square Op											
			1-1/4"	1"	3/4"	5/8"	1/2"	3/8"	1/4"	No. 4	No. 8	No. 10	No. 16	No. 30
(figures are percents by weight)														
1 Ala.	Percent passing	Total aggregate		100	75-100			60-80		40-60		20-40		
2 Ariz.	ditto	ditto		100				45-65				25-45		17
3 Ark.	Percent retained	"			0					25-45		15-60		20
4 Calif.	Percent passing	"		100	95-100			60-75		40-55	30-40			
	ditto	"		100	95-100			65-80		45-60	30-45			
5 Colo.	"	"		100	90-100					40-52	30-40			
6 Conn.	"	"	100	95-100			60-100			23-55		22-44		17
7 Del.	"	"					100	80-100		50-65		30-45		20
8 D. of C.	"	"					100	80-100		55-80		40-75		
9 Fla.	Pct. pass. & ret. 1/	"					8-39		8-45		9-27			5
10 Ga.	Percent passing	"					100	95-100		60-80			35-50	
11 Idaho	ditto	"			100					50-70		30-50		
12 Ill.	Pct. pass. and ret.	Total mixture		95-100 passing							10-30			
13 Ind.	ditto	ditto					2-14		25-50		10-30			
14 Iowa	Percent passing	Total aggregate		100	98-100		98-100	67-87		47-61	37-55			
15 Kans.	Percent retained	ditto		0	0-5			12-35			35-60			
16 Ky.	Percent passing	"					100	85-100		50-70	35-50		20-40	
17 La.	ditto	"			100					60-80		40-60		24
18 Me.	"	"					100			35-75		30-55		18
19 Md.	"	"			100	88-100		66-80		48-62		32-44		
20 Mass.	Pct. pass. and ret.	Total mixture		100 passing				25-40	6-15	15-25			4-12	
21 Mich.	ditto	ditto		100 passing					50-65					
22 Minn.	Percent passing	Total aggregate			100	98-100		70-85		50-65		35-50		
23 Miss.	ditto	ditto					100	95-100		80-95		55-75		
24 Mo.	Pct. pass. and ret.	Total mixture	100 passing		0-3		0-25		20-45		7-20		7	
25 Mont.	ditto	ditto	100 passing		15-40				10-35		8-20		10	
26 Nebr.	Percent retained	Total aggregate		0	0-4			5-30		35-55		55-75		
	ditto	ditto			0							28-38		
27 Nev.	Percent passing	"		95-100			60-80		40-55			30-50		17
28 N. H.	ditto	"					100	80-95		45-75				
29 N. J.	Pct. pass. and ret.	Total mixture	3/	-	0-25			20-45		5-25	7/-	2-14		
	ditto	ditto	3/	-	0-10			12-40		8-30	7/	2-17		
30 N. H.	Percent passing	Total aggregate			100		90-100	55-85		40-65	30-50			
31 N. Y.	Pct. pass. and ret.	Total mixture		-	0-5			15-28		20-40	8/	12-30		
32 N. C.	ditto	ditto	100 passing		0-5			30-50			10-20		8-25	
33 N. Dak.	Percent passing	Total aggregate			100				50-83			25-60		
34 Ohio	Pct. pass. and ret.	Total mixture	100 pass	-0-5		5-20	27-30		10-35	20-10		20-45		
35 Okla.	Percent passing	Total aggregate			100		20-100			55-80		40-55		12
36 Oreg.	Pct. pass. and ret.	Total mixture	100 passing				40-52				11-21			
37 Pa.	Percent passing	Total aggregate					100	80-100		45-75	30-55	20-40		
											2/			
38 R. I.	Pct. pass. and ret.	Total mixture					100-0-15	25-55		0-18		5-20		10
39 S. C.	Percent passing	Total aggregate					100	75-97		58-75		42-60		
40 S. Dak.	ditto	ditto		100	90-100		75-90		50-75			35-55		
41 Tenn.	"	"					100			64-76		46-56		
	"	"					100	95-100		65-85		45-65		
	"	"						100		85-100				
42 Texas	Pct. pr s. and ret	Total mixture			3/	100-1	77-100	75-50	1	15-35			0-2	
43 Utah	Percent passing	Total aggregate					100	90-100		70-100		60-90		
44 Vt.	ditto	ditto					100	61-92		46-84		24-71		
45 Va.	"	"					100	80-100		50-70		35-50		
46 Wash.	Pct. pass. and ret.	" 10/				0-10	30-50			20-40			30	
47 W. Va.	Percent passing	"				100	85-100			60-80	40-60			
48 Wisc.	ditto	"				95-100	75-100			45-85		30-55		
49 Wyo.	"	"					100			50-70		30-50		
50 Ontario	"	"					100	75-88	60-74	50-60	41-60	29-55		11/
	"	"										11/		
	"	"					100	92-100	77-90	64-77	55-65	45-65	33-59	

1/ Percent of material passing one sieve and retained on the next finer sieve

2/ Percent of total aggregate

3/ Round sieve openings, 1/4-in. size and larger.

4/ Passing No. 4, retained No. 6 sieve, 0-11 percent, passing No. 6 sieve, retained No. 8, 0-11 percent

5/ Maximum. Also, the No. 80 to No. 200 material shall be at least 5 percent of total aggregate

6/ Not more than 1/4 of the 1/2-in. to No. 4 fraction in the surface course shall be retained on a 3/8-in. sieve

7/ Retained on No. 10, 30-60 percent.

TABLE 6 (continued)

1954 Practice

Specified Bitumen Content of Mixture						Remarks	Agency		
No.30	No.40	No.50	No.80	No.100	No.200				
	10-25		5-15		2-8	5.0-8.0	2/	At least 4 pct. to be retained between consecutive sieves	1 Ala.
	15-25				2-10	4 0			2 Ariz.
	70-85				90-96	5.0-8.0			3 Ark.
12-22					3-6	3-7	2/	Heavy traffic	4 Calif.
15-25					3-7	3-7	2/	Medium traffic	
22-30				11-19	4-8	5 0-6 5			5 Colo.
	12-37		8-18		4-8	5.5-8.0		At least 4 pct. to be retained between consecutive sieves	6 Conn.
	15-25		10-20		5-10	5.5-8.0			7 Del.
	10-30		3-15		2-8	4.0-8 0			8 D. of C.
		9-27		5-18	5-8	5.0-9.0			9 Fla.
		15-35		10-20	7-10	6 0-10			10 Ga.
					5-12	Not specified			11 Idaho
		7-22		5-13	4-8	5.0-7.0			12 Ill.
10-25			2-17	1-5	3-5	6.5-8.5		45-55 pct. retained No. 6	13 Ind.
19-34	13-26			6+	3-10	6.25			14 Iowa
65-80		89 2/		89-94		5.0-8.0	2/		15 Kans.
	2-20		0-10	0-5	4 0-8 0				16 Ky.
	20-35	12-25		4-10	4.5-6.5				17 La.
	12-40	7-19		3-8	6.0-8 0				18 Me.
	10-20	6-14		2-8	5.0-7.0			At least 4 pct. to be retained between consecutive sieves	19 Md.
6-16		6-16	4-10	4-6	6.0-7.0			35-45 percent passing No. 10	20 Mass.
25-40				4-5	4 5-6.5				21 Mich.
	15-30		8-16		4-8	5.5-6.2		At least 4 pct. to be retained between consecutive sieves except two largest	22 Minn.
	28-42		12-24		6-10	7.2-8.7			23 Miss.
		5-20		5-18	4-10	4.0-7.0			24 Mo.
		5-20		5-15	4-8	5.0-8 5			25 Mont.
	78-88		85-93	90-95	4 5-6.0		2/	Heavy traffic	26 Nebr.
	77-87			80-95	4.5-6 0		2/	Medium traffic	
	20-27	13-20		5-11	3.0-7.0				27 Nev.
	10-30	5-20		3-8	5 5-7.5				28 N.H.
	5-18	4-18		3-16	5-8			Heavy traffic	29 N.J.
	4-24	6-22		3-20	4-8	5.5-9.0		Medium traffic	
	15-30		8-20		4-10				30 N.M.
	5-20			1-6	2-6	5.8-7.0			31 N.Y.
		7-21		4-12	2-8	5.0-7.5			32 N.C.
15-42		10-28		5-17	2-8	4.5-9.5			33 N.Dak.
			3-15		0-5	4.0-9.5			34 Ohio
	20-37		10-25		4-8	5.0-7.5			35 Okla.
10-30	3-9		3-7		3-7	5 0-7 0		At least 10 pct. ret. 1/2 inch	36 Oreg.
	5-20		2-12		2-8	5.3-8 5		6.5 to 9.5 pct. bitu. for slag	37 Pa.
		3-18		3-5	5-8	6 5-8.5			38 R.I.
25-35		15-25		5-12		6.0-7 5		At least 5 pct. to be retained between consecutive sieves smaller than 3/8 in.	39 S.C.
	20-30			6-10		5.0-7 0			40 S.Dak.
	19-27		5-11			4 5-7.5		Heavy traffic	41 Tenn.
	15-30		8-20		4-9	4.5-7.5		Medium traffic	
				0-10		5-9		Medium traffic	
		5-25		5-25	+2-10	4.0-7.5			42 Texas
	30-70		10-40		5-12	5.0-6.5			43 Utah
	19-33		10-26		5-8	6.0-8.0			44 Vt.
	10-25		3-15		2-10	5.5-8.5			45 Va.
		20-50		10-30	+5-16	4.5-7 0			46 Wash.
		7-20			1-5	6.0-10			47 W. Va.
	15-35		10-25		5-12	4 0-8.0		At least 5 pct. to be retained between consecutive sieves smaller than 3/8 inch.	48 Wisc.
					5-10	5.0-7.0			49 Wyo.
20-43	11-26		6-12	3-8		5-7	2/	Heavy traffic	50 Ontario
22-47	12-29		6-13	3-8		5-7	2/	Medium traffic	

8/ No. 6 sieve.

9/ Passing No. 4, retained No. 6 sieve, 0-8 percent, passing No. 6 sieve, retained No. 8, 0-10 percent.

10/ Percent limitations for material finer than No. 10 based on total fraction passing No. 10 Of total aggregate, 20-40 percent permitted to pass No. 10 sieve

11/ No. 14 sieve.

TABLE 7  
SPECIFIED TOLERANCES FROM JOB-MIX FORMULAS AND TYPICAL FORMULAS  
FOR BINDER-COURSE MIXTURES

Agency	Method of Specifying Sieve-Size Limits	Basis of Percentage Limits	Specified Tolerances from Job-Mix Formula																		
			Standard Sieve Size or Number - Square Openings																		
			2"	1-1/2"	1-1/4"	1"	3/4"	5/8"	1/2"	3/8"	1/4"	No. 4	No. 8	No. 10	No. 15	No. 20	No. 30	No. 40	No. 50	No. 80	No. 100
(Figures are percentages plus or minus from formula percentage)																					
1 Ala	Percent passing	Total aggregate		4	4			4	1			1		5					3		
2 Ariz									Not specified												
3 Ark	Percent retained	Ditto		+5,-7				5				+2,-1/2		5			3				
4 Calif	Percent passing	"															5				
5 Colo	Ditto	"																			
6 Conn.	"	"																			
7 Del.	"	"		7	7	7	7	7	4			4		4		4		4		4	
8 D. of C.	"	"						7						5							
9 Fla	Pct pass and ret	"						5									5				
10 Ga	Percent passing	"			7			7				5	4		4				4		2
11 Idaho	Ditto	"										Not reported								4	2
12 Ill	Pct pass and ret	Total mixture										5									
13 Ind	Ditto	Ditto						5									3				
14 Iowa	Percent passing	Total aggregate	8		8	8	8	8	8	5		5									
15 Kans	Percent retained	Ditto								2							+3,-5				
16 Ky.	Percent passing	"			4	4			4			4		5				2			
17 La	Ditto	"				7			7			7		5				5		3	
18 Me	"	"				6			6			6		4				4		3	
19 Md	"	"			7	7			7			4		4				4		4	
20 Mass	Pct pass and ret	Total mixture								Not reported											
21 Mich.	Ditto	Ditto												3							
22 Minn.	Percent passing	Total aggregate			7	7		7	7			7		7				6		5	0.2
23 Miss.	Percent passing	Total aggregate																			0.2
24 Mo.	Pct pass and ret	Total mixture			5				5			3		2				3			1.0
25 Mont	Percent passing	Total aggregate						5				5		5							0.7
26 Nebr	Percent retained	Ditto																5		3	
27 Nev	Percent passing	"								Not reported											
28 N. H.	Ditto	"					10			10		4						4			
29 N. J.	Pct pass and ret.	Total mixture										5		4							
30 N. M.	Percent passing	Total aggregate					5					5									
31 N. Y.	Pct pass and ret	Total mixture																			
32 N. C.	Ditto	Ditto																			
33 N. Dak.	Percent passing	Total aggregate																			
34 Ohio	Ditto	Ditto																			
35 Okla	Ditto	Ditto																			
36 Oreg	Pct pass and ret	Total mixture																			
37 Pa.	Percent passing	Total aggregate	5		5	10		5				4		4		4		4		4	
38 R. I.	Pct pass and ret	Total mixture																			
39 S. C.	Percent passing	Total aggregate						10		3		7		4							
40 S. Dak.	Ditto	Ditto																			
41 Tenn	"	"				7						4									
42 Tex.	Pct pass and ret	Total mixture						5		7		5		5		3					
43 Utah	Percent passing	Total aggregate				7				8		8		4		5		5		3	
44 Vt.	Ditto	Ditto																			
45 Va.	"	"				+4,-1			5		15		8		+7,-8						+2
46 Wash	"	"				7		7		4		4		4							
47 W. Va.	"	"				5				5		5		3				3			
48 Wisc	"	"																			
49 Wyo	"	"								-12+15		6		6							
50 Ontario	"	"				3/5		5		5		5				4/5				4	

1/ Percent of total aggregate

2/ Round sieve openings, 1/8 inch size and larger

3/ 7/8 inch sieve

4/ No. 14 sieve

5/ Indicated tolerances are usual working limits and are not specified

TABLE 7 (continued)

1954 Practice

Bitumen Content of Mixture	Typical Job-Mix Formula																	Remarks	Agency			
	Standard Sieve Size or Number - Square Openings																					
	2"	1-1/2"	1-1/4"	1"	3/4"	5/8"	1/2"	3/8"	1/4"	No. 4	No. 8	No. 10	No. 16	No. 20	No. 30	No. 40	No. 50			No. 60	No. 80	No. 100
(Figures are percent by weight)																						
0.4																						
0.5																						
0.2																						
0.5																						
0.4																						
0.3																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						
0.5																						



TABLE 8

SPECIFIED TOLERANCES FROM JOB-MIX FORMULAS AND TYPICAL FORMULAS  
FOR SURFACE-COURSE MIXTURES

Agency	Method of Specifying Sieve-Size Limits	Basis of Per- centage Limits	Specified Tolerances from Job-Mix Formula																		
			Standard Sieve Size or Number - Square Openings																		
			1-1/2"	1-1/4"	1"	3/4"	5/8"	1/2"	3/8"	1/4"	No 4	No 8	No 10	No 16	No 20	No 30	No 40	No 50	No 80	No 100	No 200
(Figures are percentages plus or minus from formula percentage)																					
1 Ala	Percent passing	Total aggregate							4				5								3
2 Ariz	Ditto	Ditto							Not reported												
3 Ark	Percent retained	"							5							3					2
4 Calif	Percent passing	"							6						5						3
5 Colo	Ditto	"				5				+5,-7									+5,-3	+3	-1
6 Conn	"	"							5												2
7 Del	"	"							7												2
8 D of C	"	"							7												2
9 Fla	Pct pass and ret	"							5												2
10 Ga	Percent passing	"				7				5											2
11 Idaho	Ditto	"								5											2
12 Ill	Pct pass and ret	Total mixture								Not reported											-1 1/2
13 Ind	Ditto	Ditto							3												1 1/2
14 Iowa	Percent passing	Total aggregate				8	8			8	2/3										2
15 Kans	Percent retained	Ditto							5												1 1/2
16 Ky	Percent passing	"							4												2
17 La	Ditto	"							1												2
18 Me	"	"							6												2
19 Md	"	"				7				7											2
20 Mass	Pct pass and ret.	Total mixture																			2
21 Mich	Ditto	Ditto							2												-0 5
22 Minn	Percent passing	Total aggregate							4												0 5
23 Miss	Ditto	Ditto							7												2
24 Mo	Pct pass and ret	Total mixture							1												+1
25 Mont	Ditto	Ditto								5											2
26 Nebr	Percent retained	Total aggregate								Not reported											2
27 Nev	Ditto	Ditto								5											2
28 N H	Percent passing	"								Not reported											2
29 N J	Pct pass and ret	Total mixture							10												+3,-1
30 N M	Ditto	Ditto								4											+3,-1
31 N Y	Percent passing	Total aggregate							5												3
32 N C	Pct pass and ret	Ditto								4											2
33 N Dak	Percent passing	Total aggregate								Not reported											2
34 Ohio	Pct pass and ret	Total mixture								Not reported											2
35 Okla	Percent passing	Total aggregate								Not reported											2
36 Oreg	Pct pass and ret	Total mixture								Not reported											2
37 Pa	Percent passing	Total aggregate								Not reported											2
38 R I	Pct pass and ret	Total mixture								Not reported											2
39 S C	Percent passing	Total aggregate								Not reported											2
40 S Dak	Ditto	Ditto								Not reported											2
41 Tenn	"	"								Not reported											2
42 Tex	Pct pass and ret.	Total mixture								Not reported											2
43 Utah	Percent passing	Total aggregate								Not reported											2
44 Vt.	Ditto	Ditto								Not reported											2
45 Va	"	"								Not reported											2
46 Wash	"	"								Not reported											2
47 W.Va	"	"								Not reported											2
48 Wisc	"	"								Not reported											2
49 Wyo.	"	"								Not reported											2
50 Ontario	"	"								Not reported											2

1/ Percent of total aggregate

2/ No 6 sieve

3/ Round sieve openings, 1/4 inch size and larger

4/ Five percent pass No 200 sieve for heavy traffic

5/ No 14 sieve

6/ Indicated tolerances are usual working limits and are not specified



TABLE 9

## USE OF STABILITY TESTS IN DESIGNING AND CONTROLLING BITUMINOUS CONCRETE MIXTURES

Agency	Stability Test	Limits for Test Values Included in Specifications	Limits for Test Values Used in Design Only	Stability Value			Flow			Measured Characteristics	
				Medium Traffic	Heavy Traffic	Traffic Undiffer.	Medium Traffic	Heavy Traffic (0.01")	Traffic Undiffer.	Medium Traffic	Heavy Traffic Relative De (percent of the
1 Ala.	Marshall		x	1000	1500				m		
2 Ariz.	Eveem		x			30+			12		
3 Ark	Marshall		x	500							
4 Calif.	Eveem	x				35					
5 Colo.	Marshall		x						16-		
6 Conn	Eveem		x			35					
7 Del.	Marshall		x			1500+			16-		
8 D of C.	Hubbard-Field		x			500+			20-		
9 Fla.	Hubbard-Field	x		1200	3000	1500					
10 Ga.	Asphalt Institute	x									95-98
11 Idaho	Hubbard-Field					m					
12 Idaho	Eveem		x			40+					
13 Ill.	Marshall		x	1200+	1500+		12-20	8-16			
14 Ind	Trial and Error										
15 Iowa	Eveem		x								
16 Kans.	Triaxial Compression		x								
17 Ky.	Trial and Error										
18 La.	Marshall	x				1000+			8-18		
19 Me.	Eveem	x				35-50			m		
20 Md.	Marshall		x	1000	1500						
21 Mass.	Eveem		x			35-50					
22 Mich.	Hubbard-Field										
23 Minn.	Marshall		x			500+			20-		
24 Miss	Marshall (modified)	x		200-400	400+					90+	92+
25 Mo.	Hubbard-Field	x				3000+					
26 Mont	Hubbard-Field					m					
27 Nebr.	Hubbard-Field					m					
28 Nev.	Immersion-Compression										
29 N.H.	Eveem					m					
30 N.E.	Unconfined Compression					300-400psi					
31 N.J.	Marshall		x			1500+			12-20		
32 N.M.	Trial and Error		x								
33 N.C.	Unconfined Compression		x	200+	300+						
34 N.Dak.	Immersion-Compression										
35 N.Dak.	Vibrating Table										
36 Ohio	Marshall		x			1000-1500			10-15		
37 Okla.	Hubbard-Field		x	3000-4500							
38 Oreg.	Vibrating Table		x								
39 Pa.	Eveem	x				35+					
40 R.I.	Eveem					m					
41 S.C.	Trial and Error		x								
42 S.Dak.	Hubbard-Field		x	600+	2500						
43 Tenn.	Marshall		x		2000+						
44 Tex.	Marshall		x			500+			20-		
45 Utah	Hubbard-Field		x			m			m		
46 Vt.	Eveem (modified)	x				35+					
47 Va.	Marshall		x			1000+			12-18		
48 Wash.	Hubbard-Field					m			m		
49 W.Va.	Marshall	x		500	1500				20-		
50 Wisc.	Eveem		x								
51 Wyo.	Trial and Error		x			35+					
52 Ont.	Marshall		x	1000+	1500+				16-		
53 Ont.	Direct Compression		x			200 psi					
54 Ont.	Marshall		x			1500+			15-		
55 Ont.	Triaxial Compression		x								

1/ An "m" indicates that the characteristic was reported as measured, but no limiting values were reported.

TABLE 9 (continued)

1954 Practice

and Limiting Values 1/							Specific Gravity Used in Theoretical Calculations	Miscellaneous	Agency
Traffic Undiffer.	Medium Traffic	Heavy Traffic	Traffic Undiffer	Medium Traffic	Heavy Traffic	Traffic Undiffer.			
retical							Apparent Bulk Bulk Apparent, Bulk	Cohesimeter Value 50+ Swell 0.030"±.	1 Ala. 2 Ariz. 3 Ark. 4 Calif.
			3-5						
			4-6				Bulk		5 Colo.
94-97 Max.			3-5			75-85	Vacuum Saturated Bulk Bulk		6 Conn. 7 Del. 8 D. of C 9 Fla.
m			m				Bulk Bulk		10 Ga.
			2-6				Apparent Apparent		11 Idaho 12 Ill. 13 Ind. 14 Iowa 15 Kans.
							Bulk	Cohesion 8 psi. Angle of internal friction 25° Modulus of deformation 25000 psi.	
92-96							Surface Dry		16 Ky.
92+			8- 4+				Bulk Apparent Apparent, Bulk Bulk Apparent Bulk Apparent Apparent, Bulk		17 La. 18 Mo. 19 MI. 20 Mass. 21 Mich. 22 Minn. 23 Miss. 24 Mo.
95-98			3-6				Bulk-Surface Dry Bulk		25 Mont. 26 Nebr.
			3-8				Apparent		27 Nev. 28 N.H. 29 N.J. 30 N.M. 31 N.Y.
94-98			3-5 4-8			75-85	Bulk Bulk Bulk		32 N.C.
Max.							Bulk		33 N.Dak.
94-98 m	3	5					Bulk Apparent, Bulk Apparent, Bulk		34 Ohio 35 Okla. 36 Oreg.
94-98						75-85	Apparent Apparent Effective Apparent		37 Pa. 38 R.I. 39 S.C. 40 S.Dak. 41 Tenn.
94-98			3-7			93-97	Bulk Apparent		42 Tex. 43 Utah
90 90			m			m	Surface Dry Bulk Bulk Apparent		44 Vt. 45 Va.
94-98 92 94-97			3-6			65-85	Apparent Apparent Effective	Cohesion 15 psi. Angle of internal friction by cell test, 27 + for heavy traffic.	46 Wash. 47 W.Va. 48 Wisc. 49 Wyo. 50 Ontario

TABLE 10  
BITUMINOUS CONCRETE CONSTRUCTION REQUIREMENTS - PART I

Agency	Plant									
	Aggregate Storage		Temperature Requirements			Maximum Moisture in Aggregates percent	Mixing-Time Requirements			
	Stock Piled Separately	Stock Pile Construction	Aggregate Temperature of	Asphalt Cement of	Mixture at Discharge of		Batch-Type Plant		Total	Total
							Dry sec.	Wet sec.	sec.	sec.
1 Ala.	Yes	-	225-350	Varies	225-300	0.5	Thorough	45	45	-
2 Ariz.	No	1/ N.S.	375 max.	3/ N.S.	375 max.	1.25	Thorough	30	-	Thorough
3 Ark.	Yes	In layers	350 max.	300 max.	250-325	N.S.	Thorough	30	-	30
4 Calif.	Yes	No segregation or degradation	275-350	275-350	N.S.	1.0	N.S.	30	30	N.S.
5 Colo.	Yes	N.S.	225-325	200-325	225-325	2.0	Thorough	45	N.S.	45
6 Conn.	Yes	N.S.	300-350	N.S.	265-325	N.S.	15	30	45	45
7 Del.	Yes	No segregation	325 max.	250-350	275-325	N.S.	15	45	90	-
8 D.of C.	Yes	3-ft. layers	250-400	250-350	250-350	N.S.	15	45	60	-
9 Fla.	Yes	3-ft. layers	250-340	250-340	250-340	Dry	15	45	60	60
10 Ga.	Yes	Min. 6' height	350 max.	250-350	300 max.	-	15	45	60	45
11 Idaho	No	3-ft. layers	325 max.	200-400	325 max.	1.0	-	30	30	30
12 Ill.	Yes	-	1/250-350-B 275-375-S	250-350	325 max.-B 350 max.-S	Dry	5-B 15-S	30	35-B 45-S	35-B 45-S
13 Ind.	Yes	No coning or segregation	300-375	200-300	225 min.	1.0	15	30-45	45-60	Thorough
14 Iowa	Yes	4-ft. layers	275-335	225-300	310 max.	No foaming	20	30	50	50
15 Kans.	Yes	No segregation or degradation	325 max.	275-325	225-325	No foaming	Thorough	35-B 45-S	60	N.S.
16 Ky.	Yes	-	250-325	225-325	250-300	Trace	15	30-45	40-60	-
17 La.	Yes	-	250-350	250-325	250-325	1.0	N.S.	45	45	-
18 Mo.	Yes	N.S.	250-300	275 min.	300-350	N.S.	15	55	70	-
19 Md.	Yes	4-ft. lifts	250-325	250-350	225-350	N.S.	15	45	60	-
20 Mass.	Yes	N.S.	-	275-350	250-300	N.S.	N.S.	45	N.S.	-
21 Mich.	Yes	No segregation	400 max.-B 425 max.-S	275-350	280-375	0.0	10	35-B 50-S	45-B 60-S	-
22 Minn.	Yes	No intermixing	325 max.	225-300	325 max.	Surface dry	15	25	40	40
23 Miss.	Yes	Layers	250-400	250-350	250-350	Dry	-	-	60	-
24 Mo.	Yes	No segregation	225-350	250-325	N.S.	N.S.	15	30	45	35
25 Mont.	Yes	-	225-275	225-300	225-300	N.S.	Thorough	45	-	-
26 Nebr.	Yes	3-ft. layers	250-325	250-350	275 ±20	N.S.	15	30	45	45
27 Nev.	Yes	N.S.	275-325	250-400	275-325	1.0	10	30	40	-
28 N.H.	Yes	N.S.	250-325	250-350	250-350	No foaming	-	45	45	35
29 N.J.	Yes	No segregation	225-350	250-325	325 max.	N.S.	Thorough	45	45	-
30 N.M.	No	N.S.	250-325	275 ±20	250-280	Dry	10	30	40	30
31 N.Y.	Yes	N.S.	325 max.	-	225-275	N.S.	15	30	45	-
32 N.C.	Yes	No segregation	250-375	250-325	250-350	N.S.	N.S.	45	45	-
33 N.Dak.	N.S.	No segregation	325 max.	300 max.	N.S.	Dry	15	20	35	-
34 Ohio	Yes	-	N.S.	300 max.	325 max.	Dry	15	30	45	45
35 Okla.	Yes	No intermixing	325 max.	250-300	325 max.	0.5	5	30	35	35
36 Oreg.	Yes	-	325 max.	300 max.	250-325	N.S.	Thorough	30	N.S.	-
37 Pa.	Yes	4-ft. layers	N.S.	250-325	225-325	Dry	Thorough	40	42-45	-
38 R.I.	Yes	-	300-375	250-350	275-350	N.S.	15	45	60-75	-
39 S.C.	Yes	No segregation	250-350	-	250-350	N.S.	Thorough	45	45	-
40 S.Dak.	Yes	-	-	-	235-325	1.0	-	-	35	35
41 Tenn.	Yes	No segregation	300-400	250-325	4/ 250-325 2/ 200-300	N.S.	-	-	30	40
42 Tex.	Yes	-	Varies	180-350	200-350	N.S.	5-20	30	35-50	35-50
43 Utah	No	-	250-320	250-325	250-300	-	-	30	-	-
44 Vt.	Yes	-	275-350	-	275-350	-	Thorough	45	45	-
45 Va.	Yes	5-ft. layers	225-300	225-275	225-275	0.2	15	45	60	45
46 Wash.	Yes	4-ft. layers	300-385	250-325	260-375	N.S.	-	30	-	N.S.
47 W.Va.	Yes	Preserve quality	300 max.	250-300	200-300	0.5 to 1.0	15	45	60	60
48 Wisc.	Yes	N.S.	225-350-B 275-375-S	250-350	250-350	1.0	Thorough	45	60 ±	-
49 Wyo.	No	N.S.	250-325	275-350	250-350	1.0	-	30	Thorough	30
50 Ontario	Yes	Layers	325 max	275 max	N.S.	N.S.	15	25	40	35

1/ B = binder-course material; S = surface-course material

2/ Formula

$$\text{Sec} = \frac{\text{Pugmill Dead Capacity (lbs)}}{\text{Pugmill Output (lbs./sec)}}$$

3/ N

TABLE 10, PART I (continued)

- Minimum Continuous-Type Plant How Determined	Placement								Agency
	Temperature Requirements			Spreading and Finishing Machine		Lift Thicknesses			
	Air Minimum °F.	Mixture at Placing		Operating Speed ft. per min.	Maximum Permitted		Normally Placed		
		Range °F.	Daily Tolerance °F.		Binder inches	Surface inches	Binder inches	Surface inches	
Formula 2/ Not reported Not reported	40 N.S. 35	- N.S. 250-325	N.S. N.S. ± 25	N.S. - -	- Not used 3	- 3½ 2	- Not used 2-3	- 2 1½ - 2	1 Ala. 2 Ariz. 3 Ark.
-	40	N.S.	N.S.	N.S.	2	2	1½	1½	4 Calif.
Formula	N.S.	225-325	N.S.	-	3	2	1½	1½	5 Colo.
-	60	265-325	± 25	N.S.	2	2	1½	1½	6 Conn.
Formula	40	255-305	N.S.	N.S.	2	1½	-	-	7 Del.
Formula	50	225-350	± 20	-	2	2	1½	1½	8 D. of C.
Full dead capacity - lbs.	40	250-340	± 30	7-28	2	2	1½	1	9 Fla.
Formula	40	-	-	10-20	-	-	1-2	1 - 1½	10 Ga.
-	35	200-300	N.S.	N.S.	-	2½	-	2½	11 Idaho
Formula	40	250-325-B	± 20	20-25	2	1½	1½	1½	12 Ill.
Not reported	40	250-350-S	± 20	N.S.	-	-	-	-	13 Ind.
Formula	40	225-325	± 20	N.S.	-	-	-	-	14 Iowa
-	40	250-275	± 20	35 max.	-	-	1½	1½	15 Kans.
Formula	40	225-325	N.S.	10-20	-	-	-	-	
rated capacity of plant	40	225-300	N.S.	25 max.	1½	1½	1½	1½	16 Ky.
Continuous plant not used	36	250-325	± 25	N.S.	2	2	2	2	17 La.
Formula	40	275-325	± 25	N.S.	2	1	1	1	18 Mo.
Formula	32 rising 38 falling	225-350	± 20	5-30	3	2	2	1½	19 Md.
Formula	40	250-300	± 20	N.S.	-	-	-	-	20 Mass.
Continuous plant not used	40	280-375	± 20	5-20	170 p.s.y.	130 p.s.y.	-	100 p.s.y.	21 Mich.
Formula	40	N.S.	± 20	30 max.	2½	2½	1½-2	1½-2	22 Minn.
Formula	40	225-325-B	± 25	-	-	-	1½-2½	1 - 2	23 Miss.
Formula	40	250-350-S	± 25	N.S.	2	2	1 3/4	1½	24 Mo.
Formula	40	200-350	± 25	10-20	2	2½	1½	1½-2-2½	25 Mont.
Formula	40	300 max.	± 10	10-30	-	2	-	1½	26 Nebr.
-	40	275 max.	± 20	-	-	2	-	-	27 Nev.
Formula	50	275-325	± 20	-	2	2½	-	-	28 N.H.
Formula	50	225-350	N.S.	-	3	1	2	1	29 N.J.
Continuous plant not used	40	325 max.	± 15	5-50	-	-	-	-	30 N.M.
Full output	35 rising 40 falling	225-255	± 15	20 max.	-	2	1½	2	31 N.Y.
-	50	225-275	N.S.	N.S.	1½	1	1½	1	32 N.C.
Formula	35	225-325	± 30	30 max.-B 20 max.-S	3	2	1½	1½	33 N.Dak.
Formula	35	225 min.	-	30 max.	Var.	Var.	-	2½	34 Ohio
-	40	240 min.	± 25	As required	-	1½	-	1-1½	35 Okla.
Formula	40	225-300	± 20	-	-	-	2-3	-	36 Oreg.
Formula	40	250-300	N.S.	10-50	3	3	2	1½	37 Pa.
Continuous plant not used	40	225-300	± 15	-	3	1	2-3	1	38 R.I.
Formula	40	250-375	± 20	Avoid tearing	1½	1½	1½	1½	39 S.C.
Formula	35	250-350	± 20	-	-	-	-	-	40 S.Dak.
Capacity of mixer, drier and belt pump	40	250-325	± 10	30 max.	1-1½	2	1-1½	1½	
Formula	40	4/225-300 5/175-275	± 20	-	-	-	2½	1½	41 Tenn.
Not reported	N.S.	N.S.	± 30	-	-	3	-	1	42 Tex.
Formula	50	250-300	-	-	1½-2	1-1½	1½	1½	43 Utah
Formula	40	275-325	± 25	-	1½	1-1½	1½	1	44 Vt.
Formula	40	225-275	± 20	10-30	2	1½	2	1	45 Va.
-	35	250 min.	-	-	3	-	1-3	-	46 Wash.
Observation	45	200-300	± 20	-	-	-	-	-	47 W.Va.
Formula	50	225-325-B	± 20	20 max.	1½	1½	1½	1½	48 Wisc.
Formula	40	250-350-S	N.S.	Avoid tearing	1½	2	1½	1½	49 Wyo.
Formula	45	250-350	N.S.	10-20	2½	1½	2	1½	50 Ontario

Specified in specifications.

4/ Stone.

5/ Gravel.

TABLE 10  
BITUMINOUS CONCRETE CONSTRUCTION REQUIREMENTS - PART II

Agency	Compaction				
	Rolling Requirements				Maximum Roller Speed mph
	Max Tons Per Roller-Hour	Minimum Num- ber of Rollers	Roller Types 5/	Other Requirements	
1 Ala.	30	2	T or W		2
2 Ariz.	2/ N.S.	N.S.	T or P		N.S.
3 Ark.	50	N.S.	T or W		-
4 Calif.	100	N.S.	T, P, or W		N.S.
5 Colo.	-	2	T and W		N.S.
6 Conn.	25	1	T and W	First roller tandem, additional rollers 3-wheel	3
7 Del.	40	2	T and W		N.S.
8 D.of C.	-	2	T		1.5
9 Fla.	-	2	T	One roller per 450 s.y. per hr.	N.S.
10 Ga.	N.S.	N.S.	T or W		3
11 Idaho	75	1	T		N.S.
12 Ill.	-	2	T and W	One tandem and one 3-wheel for 75 ton/hr. or less; additional rollers tandem	1.8
13 Ind.	-	2	T and W	One 3-wheel to two tandem max. ratio	N.S.
14 Iowa	40	2	T and W	Only one 3-wheel roller per job	N.S.
15 Kans.	N.S.	N.S.	T or W		1.5
16 Ky.	25	2	T or W	Only one 3-wheel roller per job	N.S.
17 La.	50	N.S.	T or W		N.S.
18 Me.	N.S.	N.S.	T	Initial rolling with 2-axle tandem, final with 3-axle tandem; not over 200 s.y. per roller per hr.	N.S.
19 Md.	-	N.S.	T	One roller per 300 s.y. per hr; 2-axle or 3-axle tandem only.	3
20 Mass.	37½	N.S.	N.S.		N.S.
21 Mich.	-	2	T	Two rollers for each spreader	N.S.
22 Minn.	50	2	T and W		3
23 Miss.	35	N.S.	T or W		3
24 Mo.	To obtain finish	2	T or W	Tandem roller preferred	3
25 Mont.	80	2	T and W		3
26 Nebr.	40	N.S.	T and W		3
27 Nev.	-	N.S.	T	Require 3-axle tandem	-
28 N.H.	-	N.S.	T	Final rolling by 3-axle tandem	N.S.
29 N.J.	-	2	T and W	One roller per 1000 s.y. per hr.	3
30 N.M.	50	3	T, W and P	Two of three to be steel-tired	Avoid displacement
31 N.Y.	25	N.S.	T or W		3
32 N.C.	-	N.S.	T	One roller per 1000 s.y. per hr.	3
33 N.D.	-	2	T or W	Must obtain required finish	3
34 Ohio	30	2	T and W		2.5
35 Okla.	-	2	T, W and P	Pneumatic rollers permitted in excess of two	N.S.
36 Oreg.	75	N.S.	T or W		Avoid displacement
37 Pa.	30	2	T and W	Additional rollers shall be 3-wheel	Avoid displacement
38 R.I.	100	2	T and W		N.S.
39 S.C.	N.S.	N.S.	T		Avoid displacement
40 S.D.	-	2	T or W	One tandem and one 3-wheel required per spreader	3
41 Tenn.	-	2	T and W	One roller per 500 s.y. per hr.	N.S.
42 Tex.	-	2	T and W	One tandem and one 3-wheel, or one 2-axle and one 3-axle tandem	N.S.
43 Utah	40	N.S.	T, W and P		N.S.
44 Vt.	150	1	T	Additional roller per 200 tons per hr.	3
45 Va.	35	2	T and W		Avoid displacement
46 Wash.	-	2	T or W	Two rollers for each spreader	Avoid displacement
47 W.Va.	30	N.S.	T or W		-
48 Wisc.	30	N.S.	T or W		1.7
49 Wyo.	40	3	T, W or P	Must include one 3-axle tandem. Add roller for each 40 tons/hr. over 160.	Avoid displacement
50 Ontario	40	2	T or W		3

- 1/ Type of specific gravity of aggregates used in theoretical calculation of density of voidless mass.  
 A - Apparent specific gravity.  
 B - Bulk specific gravity  
 S - Bulk, surface dry specific gravity  
 V - Vacuum saturated

2/ Not specified in specifications.

3/ Not specified, but considered desirable.

4/ Percentage values selected for each project individually. Relative densities (voidless, apparent specific gravity)

5/ T = Tandem, W = 3 wheel, P = Pneumatic.

TABLE 10, PART II (continued)

1954 Practice

Density Requirements			Other Required		Agency
Relative Density		Density upon Which Percentage Requirements are Based	Surface Smoothness		
Binder percent	Surface percent		Binder	Surface	
85 2/ N.S.	90 N.S.	Voidless - A 1/	1/4"-10'	1/4"-10'	1 Ala.
-	-	-	-	1/4"-10'	2 Ariz.
3/ 97+	3/ 97+	Voidless - A	3/8"-10'	1/4"-10'	3 Ark.
95+	95+	Voidless - B 1/	N.S.	1/8"-10'	4 Calif.
3/93-96	3/93-96	Voidless - V 1/	1/8"-10'	1/4"-10'	5 Colo.
-	-	-	N.S.	1/4"-10'	6 Conn.
N.S.	90+	Voidless - A	1/4"-16'	1/4"-16'	7 Del.
95+	95+	Voidless - B	N.S.	3/16"-10'	8 D. of C.
95+	95+	Hubbard-Field compacted specimen	1/4"-10'	1/4"-10'	9 Fla.
N.S.	N.S.	-	3/8"-10'	1/4"-10'	10 Ga.
95+	95+	Voidless - A	N.S.	1/4"-10'	11 Idaho
-	-	-	1/4"-10'	1/8"-10'	12 Ill.
98	98	Not stated	1/4"-10'	1/8"-10'	13 Ind.
88+	90+	Voidless - B	1/4"-10'	1/8"-10'	14 Iowa
N.S.	N.S.	-	1/4"-10'	3/16"-10'	15 Kans.
98	98	Marshall compacted specimen	1/16"-1'	1/8"-10'	16 Ky.
94-98	94-98	Voidless - A	3/16"-10'	3/16"-10'	17 La.
-	-	-	1/2"-20'	1/4"-20'	18 Me.
92+	92+	Voidless - A	1/8"-10'	1/8"-10'	19 Md.
92+	92+	Voidless - B	-	1/4"-16'	20 Mass.
N.S.	N.S.	-	1/4"-10'	1/4"-10'	21 Mich.
N.S.	N.S.	-	N.S.	3/16"-10'	22 Minn.
4/	4/	Marshall compacted specimen	1/8"-10'	1/8"-10'	23 Miss.
94-97	94-97	Voidless - A, B	1/4"-10'	1/8"-10'	24 Mo.
95-98	95-98	Voidless - S	1/2"-10'	3/16"-10'	25 Mont.
3/91-92	3/91-92	Voidless - B	-	3/16"-10'	26 Nebr.
90	90	Not stated	-	-	27 Nev.
3/ 95+	3/ 95+	Voidless - A	1/4"-10'	1/4"-10'	28 N.H.
N.S.	N.S.	-	-	3/16"to 1/8"-10'	29 N.J.
-	92-96	Voidless - A	3/16"-10'	3/16"-10'	30 N.M.
N.S.	N.S.	-	1/4"-16'	1/4"-16'	31 N.Y.
95+	95+	Voidless - B	1/4"-10'	1/4"-10'	32 N.C.
N.S.	N.S.	-	1/4"-10'	1/4"-10'	33 N.D.
-	90-95	Voidless - B	1/4"-10'	-	34 Ohio
92+	92+	Voidless - A, B	3/16"-10'	3/16"-10'	35 Okla.
92+	92+	Voidless - A	1/10"-10'	1/10"-10'	36 Oreg.
3/ 95+	3/ 95+	Voidless	Flex. base 1/4"-16'	Flex. base 1/4"-16'	37 Pa.
-	94	Hubbard-Field compacted specimen	Rigid base 1/8"-16'	Rigid base 1/8"-16'	38 R.I.
N.S.	N.S.	-	-	-	39 S.C.
N.S.	N.S.	-	N.S.	1/8"-10'	40 S.D.
3/85-90	3/85-90	Voidless-A (flexible, 85 percent; rigid, 90 percent)	1/4"-12'	1/4"-12'	41 Tenn.
3/91-96	3/91-96	Voidless - A	1/4"-16'	1/4"-16'	42 Tex.
92+	92+	Voidless - A	N.S.	1/8"-10'	43 Utah
95-99	95-99	Marshall compacted specimen	N.S.	1/4"-16'	44 Vt.
90+	90+	Voidless - A	1/4"-16'	1/8"-16'	45 Va.
N.S.	N.S.	-	N.S.	1/8"-10'	46 Wash.
-	-	-	-	1/8"-10'	47 W.Va.
N.S.	N.S.	-	N.S.	1/4"-10'	48 Wisc.
3/ 95	3/ 95	Voidless	1/4"-10'	1/4"-10'	49 Wyo.
N.S.	N.S.	-	1/8"-10'	1/8"-10'	50 Ontario

gravity) of 92+ percent for heavy traffic and 90+ percent for medium traffic.



TABLE 11  
BITUMINOUS CONCRETE EQUIPMENT REQUIREMENTS - PART I

Agency	Equipment Used in Storing and Feeding Cold Aggregates							
	Equipment Used in Convey- ing Aggregate to Cold Bins	Requirements for Cold-Aggregate Bins		Mechanical Feeder Required	Type of Feeder Normally Used	Requirements for Feeders		
		Minimum Number of Compartments	Minimum Capacity			Adjustable for Proportional Feed	Adjustable for Total Feed	Requirements for Control
1 Ala.	Clamshell	3	Supply full mixer capacity	Yes	Combination	Yes	Yes	Produce prop
2 Ariz.	N S 1/	N S	-	No	-	-	-	N S
3 Ark.	Clamshell	N S	N S	Yes	Combination	No	Yes	Produce prop
4 Calif.	Gravity belt and tunnel	2	N S	Yes	Individual	Yes	Yes	-
5 Colo.	N S.	N S	N S.	Yes	Combination	Yes	Yes	N S
6 Conn.	N S	N S	-	Not required, but used	Compartment	Yes	Yes	N S
7 Del.	Clamshell	N S.	Supply plant-rate	No	Compartment	-	-	-
8 D. of C.	-	-	-	Yes	Compartment	Yes	Yes	-
9 Fla.	Clamshell	N S	-	Yes	Combination	Yes	Yes	Produce prop
10 Ga.	Dragline	2	Not less than 3x dead-load capacity of mixer	Yes	Compartment	Yes	Yes	Produce prop
11 Idaho	Bulldozer	-	-	No	-	No	No	N S
12 Ill.	Crane and elevator	3	-	Yes	Compartment	Yes	Yes	Feed a mini to proper p
13 Ind.	Elevator	3+	-	Yes	-	Yes	Yes	Produce prop
14 Iowa	-	-	Suppl. plant-rate	Yes	-	Yes	-	Adjustable
15 Kans.	Clamshell	N S	-	Yes	Combination	Yes	Yes	Produce prop
16 Ky.	Clamshell	2	Supply plant-rate	Yes	Combination	Yes	-	Feed a mini to proper p
17 La.	Dragline and conveyor belt	One for each aggregate size	N.S.	Yes	Compartment	Yes	Yes	N.S.
18 Me.	Clamshell	2	Supply plant-rate	Yes	Compartment	Yes	Yes	Adjustable
19 Md.	N.S.	One for each aggregate size	Supply full mixer capacity	Yes	Compartment	Yes	Yes	Feed throug
20 Mass.	N S.	-	-	Yes	Compartment	Yes	Yes	Adjustable
21 Mich.	Power shovel and conveyor	-	-	Yes	Compartment	Yes	Yes	Adjustable
22 Minn.	Conveyor belt	-	N S.	Yes	Reciprocating gate feeder	Yes	Yes	Positive co
23 Miss.	Crane or belt conveyor	Varies as to type of mixture	Supply full mixer capacity	Yes	Compartment	Yes	Yes	Accurate m
24 Mo.	N.S.	One for each aggregate size	N S.	Yes	Individual	Yes	Yes	Produce pro
25 Mont.	Conveyor belt	-	Supply full mixer capacity	Yes	Combination	Yes	Yes	Uniform fee
26 Nebr.	Clamshell	One for each aggregate size	N.S.	Yes	Compartment	Yes	Yes	No locking specified h
27 Nev.	Belts	-	-	Yes	Individual	Yes	-	-
28 N.H.	Trucks	-	-	Yes	Compartment	Yes	Yes	N.S.
29 N.J.	N.S.	One for each aggregate size	-	Yes	Compartment	Yes	Yes	Accurate M
30 N.M.	-	-	-	Yes	Combination (apron type)	-	-	Positive co calibrated
31 N.Y.	N.S.	N.S.	-	Yes	Compartment	Yes	Yes	Produce pr
32 N.C.	N.S.	One for each aggregate size	Supply full mixer capacity	Yes	Reciprocating or vibrating	Yes	Yes	Accurate s total & pr
33 N.Dak.	Mechanical means	One for each aggregate size	No less than 3x dead-load capacity of mixer	Yes	Combination	Yes	Yes	Accurate
34 Ohio	Clamshell or truck	2	-	Yes	Compartment	Yes	Yes	Produce pr
35 Okla.	Bulldozers or clamshell	One for each aggregate size	In excess of mixer capacity	Yes	Compartment	Yes	-	Accurate m
36 Oreg.	Separate tunnels	3	-	Yes	Individual	Yes	Yes	Positive v
37 Pa.	Clamshell	2+	-	Yes	Individual	Yes	Yes	Accurate m
38 R.I.	Belt and bucket conveyor	-	-	Yes	Compartment	Yes	Yes	Controlled
39 S.C.	-	-	-	Yes	Compartment	Yes	Yes	-
40 S.Dak.	Conveyor	-	-	Yes	Individual	-	-	Produce pr
41 Tenn.	Clamshell and conveyor belt	-	-	Optional	Combination	-	-	Accurate m
42 Tex.	Clamshell	3+	-	Yes	Compartment	Yes	-	Feed from compartment
43 Utah	-	N.S.	Supply plant-rate	Yes	Compartment	-	-	Satisfacto feeder
44 Vt.	Crane	2	Supply plant-rate	Yes	Compartment	Yes	Yes	-
45 Va.	Clamshell	2	Supply plant-rate	Yes	Compartment	Yes	Yes	Uniform fe
46 Wash.	Belt and elevator	-	-	Yes	Individual	Yes	Yes	N
47 W. Va.	Mechanical	2	-	No	Compartment	-	-	Uniform fe
48 Wisc.	Clamshell and bulldozer	N S.	-	Yes	Compartment	Yes	Yes	Uniform fe
49 Wyo.	Bucket elevators	-	-	No	Compartment	-	-	Produce pr
50 Ontario	N.S.	3	3x mixer capacity	Yes	Compartment	Yes	Yes	-

1/ Not specified in specifications.

TABLE 11, PART I (continued)

1954 Practice

	Requirements for Aggregate Screens				
nts	Scalping Screen Opening Related to Maximum Aggregate Size	Required Capacity of Screens	Screening Efficiency (Tolerances in Specified Bin Sizes)	Agency	
proportions	1/4 in larger	In excess of mixer capacity	Not specified	1 Ala	
proportions	1/8 in larger	N S	Not specified	2 Ariz	
proportions	1/8 in larger	N S	Not specified	3 Ark	
	1/4 in larger	Prevent overflow	Not more than 10 pct undersize material in any one bin Maximum variation per day 6 pct on No 4 sieve, 5 pct on No 30 sieve, 3 pct on No 200 sieve	4 Calif	
	N S	N S	Not specified	5 Colo	
	No scalping screen	In excess of mixer capacity	Not specified	6 Conn	
	1/8 in larger	In excess of mixer capacity	Not specified	7 Del.	
	1/4 in larger	Synchronized with speed of plant	Not more than 5 pct in any bin larger than top-size screen for bin, not more than 20 pct in intermediate-size aggregate bin smaller than bottom-size screen for bin, not more than 10 pct in large-size aggregate bin smaller than bottom-size screen for bin	8 D of C	
proportions	1/8 in larger	In excess of mixer capacity	Not specified	9 Fla	
proportion	1/4 in larger	In excess of mixer capacity	No carryover	10 Ga	
of 3 sizes ations	N S	N S	Maximum carryover of 8 percent	11 Idaho	
	1/2 in larger	-	Size No 1 90+ pct pass No 10 sieve Size No 2 95+ pct pass 1/2-in sieve, 15- pct pass No 10 sieve Size No 3 95+ pct pass 1-in sieve, 15- pct pass 1/2-in sieve	12 Ill	
proportions	-	In excess of mixer capacity	Not more than 5 pct in any bin larger than designated top size, not more than 10 pct in No 2 bin to pass No 6 sieve, not more than 20 pct in No 3 bin to pass 1/2 in sieve	13 Ind	
18	No larger	In excess of mixer capacity	Not specified	14 Iowa	
proportions	N S	In excess of mixer capacity	Not specified	15 Kans	
of 3 sizes ations	1/16-1/4 in larger	-	Not more than 5 pct in any bin larger than top-size screen for bin, not more than 5 pct in No 2 bin passing top-size screen for No 1 bin, not more than 10 pct in No 3 bin passing top-size screen for No 2 bin, not more than 15 pct in No 4 bin passing top-size screen for No 3 bin	16 Ky	
es	1/4 in larger	N S	Not specified	17 La	
separate bins	1/4 in larger	125 pct of plant rated capacity	Not specified	18 Me	
	1/8 in larger	In excess of mixer capacity	Efficiency of 85 percent, based on laboratory sieves	19 Mi	
es	-	Min of 50 ton/hr	Not specified	20 Mass	
ol	1/8 in larger	In excess of mixer capacity	Tolerance of 10 percent, maximum of 5 pct ret No 10 sieve for sand	21 Mich	
	1/8 in larger	N S	Not specified	22 Minn	
nical feeder	1/8 in larger	In excess of pro- duction requirement	Not specified	23 Miss	
proportions	-	In excess of mixer capacity	Efficiency of 85 percent, based on laboratory sieves	24 Mo.	
	-	In excess of mixer capacity	Not specified	25 Mont	
ices As ngineer	1/8 in larger	Prevent interrup- tion of plant production	Not specified	26 Nebr	
	-	In excess of mixer capacity	Not specified	27 Nev	
nical feeder	N S	Min of equivalent to mixer capacity	Not specified	28 N H	
ol	No larger	In excess of mixer capacity	Not specified	29 N J	
proportions	1/4 in larger	In excess of mixer capacity	Maximum carryover of 10 percent	30 N M	
tsments for tional feed	1/16-1/8 in larger	In excess of mixer capacity	Not specified	31 N Y	
nical feeder	1/8 in larger	In excess of mixer capacity	Not specified	32 N C	
proportions	No scalping screen	N S	Not specified	33 N Dak	
	-	-	Bin No 1 5 pct max retained No 6 sieve Bin No 2 10 pct max retained 1/2- in sieve, 15 pct max pass No 6 sieve Bin No 3 5 pct max retained 1-in sieve, 25 pct max pass 1/2-in sieve Bin No 4 0 pct retained 2-in sieve, 25 pct max pass 1-in sieve	34 Ohio	
nical feeder	1/16-1/4 in larger	In excess of mixer capacity	Bin No 1 mineral filler Bin No 2 90-100 pct pass No 10 sieve Bin No 3 85-100 pct retained No 10 sieve, 85-100 pct pass 1/2-in sieve Bin No 4 85-100 pct retained 1/2-in. sieve, 100 pct pass topsize sieve	35 Okla	
e control	1/8 in. larger	In excess of plant production	Not specified	36 Oreg.	
nical feeder	N S	Meet ASTM-D-995-51	Efficiency of 85 percent, based on laboratory sieves	37 Pa.	
ed	N S	-	Not specified	38 R I	
proportions	1/8-1/4 in larger	-	Not specified	39 S C	
	No scalping screen	Equal to output of drier	Not specified	40 S Dak	
nical feeder	-	In excess of mixer capacity	Not specified	41 Tenn	
rate	N S	In excess of mixer capacity	Efficiency of 85 pct based on laboratory sieves, except that at least 90 pct of material in fine-size bin must pass No 10 sieve	42 Tex.	
mechanical	N S	In excess of mixer capacity	Not specified	43 Utah	
	1/8 in. larger	In excess of plant capacity	Not specified	44 Vt.	
	1/16 in larger	Prevent interruption of plant production	No 2 Bin not more than 10 pct. undersize No 3 bin not more than 15 pct undersize No 4 bin not more than 20 pct undersize	45 Va.	
	1/16-1/8 in larger	300 tons per day	Plus or minus 10 pct. undersize or oversize for screen used	46 Wash	
	1/2 in larger	N S	Not specified	47 W Va	
proportions	N S	In excess of mixer capacity	Not specified	48 Wisc.	
	N S	In excess of mixer capacity	Not specified	49 Wyo.	
	N S	N S	Not specified	50 Ontario	

TABLE 11  
BITUMINOUS CONCRETE EQUIPMENT REQUIREMENTS - PART II

Agency	Equipment Used During Processing of Hot Aggregate										Storage and Heating of Bitumen		
	Requirements for Hot-Aggregate-Mix			Thermometric Equipment for Aggregates							Required Capacity of Storage Tank	Type of Instrument Used	
	Number of Compartments	Binder	Surface	Minimum Capacity	Type of Instrument Permitted		Recording Instrument Required	Number of Terminals		Required Instrument Sensitivity and Efficiency			
					Pyro-meter	Thermo-meter		Single Drier	Dual Drier				
1 Ala	3		3	Supply full mixer capacity	Yes	Yes	No	4	5	-	One day's run	No	Yes
2 Ariz	-		2	N S 1/	Yes	Yes	No	N S	N S	-	N S	-	-
3 Ark	3+		3+	N S	Yes	Yes	No	1	-	-	N S	No	Yes
4 Calif	3		3	N S	Yes	Yes	No	N S	N S	100°F in one minute	N S	No	Yes
5 Colo	3		-	N S	Yes	Yes	Yes	N S	N S	N S	N S	N S	N S
6 Conn	3		3	Min. of 25 ton per hour-supply full mixer capacity	Yes	No	No	N S	N S	N S	10 hours operation	No	Yes
7 Del	4		3	Supply plant-rate	Yes	Yes	Yes	N S	N S	N S	One day's run	No	Yes
8 D of C	3		3	-	Yes	Yes	No	1	1	-	-	No	Yes
9 Fla	2		3	Supply full mixer capacity	Yes	Yes	Yes	1	2	N S	One day's run	No	Yes
10 Ga.	2+		2+	Not less than 3 times dead-load capacity of mixer	Yes	Yes	No	1	2	-	One day's run	No	Yes
11 Idaho	-		3	N S	Yes	Yes	No	N S	N S	N S	N S	No	Yes
12 Ill	3		3	Min. capacity of 6 tons	Yes	Yes	Yes	2	3	N S	One day's run	No	Yes
13 Ind	3		3	-	Yes	Yes	Yes	-	-	-	One day's run	No	Yes
14 Iowa	3+		3+	Supply plant-rate	Yes	Yes	Yes	-	-	-	One day's run	No	Yes
15 Kans	3		3	3 times mixer capacity	Yes	Yes	Yes	3	3	100°F in 15 minutes	N S	No	Yes
16 Ky	3		3	Supply plant-rate	Yes	No	Yes	1	1	N S	One day's run	No	Yes
17 La	3+		3+	N S	Yes	Yes	Yes	1	1	N S	N S	No	Yes
18 Me	3		4	Supply plant-rate	Yes	Yes	No	1	2	N S	Min. 10,000 gal	No	Yes
19 Md	3+		3+	Supply full mixer capacity	Yes	Yes	No	1	2	N S	N S	-	-
20 Mass	-		-	-	Yes	No	No	-	-	-	Min. 1,000 gal	Yes	Yes
21 Mich	2		2	10 times mixer capacity	Yes	No	No	1	1	100°F in one minute	One day's run	No	Yes
22 Minn	3		3	N S	Yes	Yes	No	N S	N S	-	N S	No	Yes
23 Miss	Varies as to type of mixture			Supply full mixer capacity	Yes	Yes	No	N S	N S	N S	N S	No	Yes
24 Mo	3+		3+	N S	Yes	Yes	No	-	-	-	Min. of 2 tanks if delivered by truck	No	Yes
25 Mont	2		3	Supply full mixer capacity	Yes	Yes	Yes	1	2	N S	One day's run	Yes	Yes
26 Nebr	2+		2+	N S	Yes	Yes	No	1	-	N S	N S	No	Yes
27 Nev	3		3	-	Yes	Yes	No	1	-	-	N S	No	Yes
28 N H	3+		3+	-	Yes	Yes	No	-	-	-	N S	No	Yes
29 N J	3+		3+	Supply plant-rate	Yes	Yes	No	1	2	-	One day's run	No	Yes
30 N M	2		3	-	Yes	Yes	Yes	1	-	-	One day's run	No	Yes
31 N Y	4		4	Not less than 3 times dead-load capacity of mixer	Yes	Yes	No	1	-	N S	N S	-	-
32 N C	3		3	Supply full mixer capacity	Yes	Yes	Yes	1	-	As directed	One day's run	No	Yes
33 N Dak	One for each size aggregate used			Not less than 3 times dead-load capacity of mixer	Yes	Yes	Yes	N S	N S	N S	One day's run	No	Yes
34 Ohio	-		3	-	Yes	Yes	Yes	1	1	-	One day's run	No	Yes
35 Okla	3+		3	Supply plant-rate	Yes	Yes	No	N S	N S	N S	One day's run	No	Yes
36 Oreg	3		3	Supply plant-rate	Yes	Yes	No	-	-	-	Provide continuous operation	No	Yes
37 Pa	3+		2+	-	Yes	Yes	Yes	1	1 to 2	-	N S	No	Yes
38 R I	4		4	-	Yes	Yes	Yes	1	-	-	N S	No	Yes
39 S C	2+		2+	-	Yes	Yes	No	1	2	-	One day's run	No	Yes
40 S Dak	3-		3-	-	Yes	Yes	No	1	-	100°F	Provide continuous operation	No	Yes
41 Tenn	3+		3+	Supply plant-rate	Yes	Yes	Yes	N S	N S	N S	ditto	No	Yes
42 Tex	4+		4+	-	Yes	Yes	Yes	N S	N S	N S	N S	No	Yes
43 Utah	3		3	Supply plant-rate	Yes	Yes	Yes	1	2	N S	Provide continuous operation	No	Yes
44 Vt	3		3	Supply plant-rate	Yes	Yes	Yes	1+	-	-	In excess of plant capacity	No	Yes
45 Va	3		3	Supply plant-rate	Yes	Yes	Yes	1	2	N S	One day's run	No	Yes
46 Wash	3		3	-	Yes	Yes	Yes	1+	1+	-	N S	No	Yes
47 W Va	3		2	-	Yes	Yes	Yes	1	-	N S	Min. 500 gal	No	Yes
48 Wisc	3		2+	N S	Yes	Yes	No	1	2	N S	N S	No	Yes
49 Wyo	3		3	Supply plant-rate	Yes	Yes	Yes	N S	N S	-	One day's run	No	Yes
50 Ontario	3		3	3 times mixer capacity	Yes	No	Yes	1	N S	N S	One day's run	No	Yes

1/ Not specified in specifications

TABLE 11, PART II (continued)

1994 Practice

Type of Material Equipment	Required Instrument Sensitivity	Requirements for Mixing Plants										Agency
		Type of Mixing Plant				Aggregate Weighing Equipment (Batch Plant)		Measuring Bituminous Material (Batch Plant)				
		Permitted		Normally Used		Type Used	Required Accuracy	Metered by Volume	Measured by Weight			
		Batch	Contin- uous	Batch	Contin- uous				Required Type of Equipment	Required Minimum Weigh-Bucket Capacity		
No	-	x	x	x		Multiple beam, springless dial	0.5 pct of max load		x	Beam or springless dial	10 pct of mixer capacity	1 Ala.
-	-	x	x	x	x	NS	NS		x	Spring-type scales	NS	2 Ariz.
No	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of max load		x	Springless dial	NS	3 Ark.
No	-	x	x	x		ditto	Not greater than 2 pct for any setting nor 1.5 pct for any batch		x	Springless dial	NS	4 Calif.
No	-	x	x		x	Scales	0.5 pct of load		x	Recording scales	NS	5 Colo.
No	-	x	x	x		Multiple beam or springless dial	0.5 pct of load	x	x	Scales	15 pct of aggregate weight	6 Conn.
No	NS	x	x	x		ditto	0.4 pct through load range		x	Beam or springless dial	Not greater than twice wt of matrl. to be weighed	7 Del.
No	-	x	x	x	x	ditto	0.5 pct or less of load	x	x	-	-	8 D of C
No	-	x	x	x	x	ditto	0.5 pct of max load		x	Beam or springless dial	-	9 Fla.
No	-	x	x	x		ditto	0.5 pct of load	x	x	Scales	20 pct of aggregate weight	10 Ga.
No	NS	x	x	x	x	Springless dial	15 pounds	x	x	Springless dial	Sufficient for one batch	11 Idaho
No	-	x	x	x		ditto	0.4 pct of weigh--hopper load	x	x	Springless dial	10-20 pct of mixer capacity	12 Ill.
No	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of true weight of load	x	x	-	15 pct of aggregate weight	13 Ind.
-	-	x	x	x	x	ditto	0.5 pct of max load, 15 lbs	x	x	-	-	14 Iowa
No	-	x	x	x	x	ditto	1.0 pct of max load	x	x	Beam or springless dial	20 pct of mixer capacity	15 Kans.
No	-	x	x	x	x	ditto	0.4 pct of max load	x	x	-	12 pct of max mixer capacity	16 Ky.
No	-	x	x	x		ditto	0.5 pct of load	x	x	-	NS	17 La.
-	-	x	x	x		ditto	0.5 pct of max load	x	x	-	25 pct of rated capacity	18 Mo.
-	-	x	x	x	x	ditto	0.5 pct of max load	x	x	Scales	15 pct of mixer capacity	19 Md.
No	-	x	x	x		Springless dial	0.5 pct of max load	x	x	-	10 pct of mixer capacity	20 Mass.
No	-	x	x	x		ditto	1/2-lb min gradation	x	x	Springless dial	Sufficient for one batch	21 Mich.
No	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of net load	x	x	Beam or springless dial	NS	22 Minn.
No	-	x	x	x	x	ditto	0.5 pct of load		x	Beam or springless dial	Sufficient to charge mixer at max capacity	23 Miss.
No	-	x	x	x	x	ditto	0.4 pct of net load	x	x	-	15 pct of mixer capacity	24 Mo.
Yes	NS	x	x	x		ditto	0.5 pct of load		x	Beam or springless dial	Sufficient for one batch	25 Mont.
No	-	x	x	x	x	Hopper & scales	NS		x	Beam or springless dial	NS	26 Nebr.
No	-	x	x	x		Multiple beam, springless dial	0.5 pct of load		x	Scales	NS	27 Nev.
No	-	x	x	x		Standard makes	Approved	x	x	Scales	Sufficient for one batch	28 N.H.
No	-	x	x	x		Weigh box or hopper suspend- ed on scale	Approved	x	x	Beam or springless dial	Sufficient for one batch	29 N.J.
No	-	x	x	x	x	Springless dial	0.5 pct of load		x	Scales	-	30 N.M.
-	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of max load	x	x	Scales	NS	31 N.Y.
No	-	x	x	x	x	ditto	0.5 pct of max load	x	x	Scales	NS	32 N.C.
No	-	x	x	x	x	ditto	± 20 pounds	x	x	-	20 pct of aggregate weight	33 N.Dak.
No	-	x	x	x		Springless dial	-	x	x	-	-	34 Ohio
No	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of max load	x	x	Beam or springless dial	15 pct of mixer capacity	35 Okla.
No	-	x	x	x		ditto	0.5 pct of max load	x	x	-	NS	36 Oreg.
No	-	x	x	x		ditto	-	x	x	Beam or springless dial	11 pct of mixer capacity	37 Pa.
No	NS	x	x	x		Springless dial	NS		x	Beam or springless dial	10 pct of mixer capacity	38 R.I.
No	-	x	x	x	x	Multiple beam, springless dial	0.5 pct of load		x	-	NS	39 S.C.
No	-	x	x	x		ditto	250 lbs per batch		x	-	20 pct of mixer capacity	40 S.Dak.
No	NS	x	x	x		ditto	0.5 pct of total load	x	x	Scales	20 pct of mixer capacity	41 Tenn.
Yes	NS	x	x	x		ditto	0.4 pct of net loads	x	x	Springless dial, cylinder	NS	42 Tex.
No	Satisfactory	x	x	x		ditto	0.5 pct of total load		x	Beam or springless dial	NS	43 Utah
No	As required	x	x	x	x	Weigh box or hopper or scales	NS		x	-	-	44 Vt.
No	-	x	x	x	x	Multiple beam, springless dial	22 lbs		x	springless dial	12 pct of mixer capacity	45 Va.
No	-	x	x	x	x	ditto	0.5 pct of max load	x	x	Beam or springless dial	Not greater than twice wt of matrl. to be weighed	46 Wash.
No	-	x	x	x	x	ditto	0.5 pct of max load	x	x	-	10 pct of mixer capacity	47 W.Va.
No	-	x	x	x	x	ditto	0.5 pct of max load	x	x	Beam or springless dial	NS	48 Wisc.
Yes	NS	x	x	x	x	ditto	1/2 of min gradation		x	Beam or springless dial	Adequate	49 Wyo.
No	-	x	x	x	x	ditto	0.5 pct of max load		x	-	20 pct of agg weight	50 Ontario

TABLE 11  
BITUMINOUS CONCRETE EQUIPMENT REQUIREMENTS - PART III

Agency	Requirements for M					
	Pugmill Mixer (Batch Plant)					Timing Device Lock Minimum Used Interval sec.
	Type of mixer Normally Used	Permissible Minimum Capacity of Mixer lbs.	Mixer-Blade Rotation Rate rpm	Max. Allowable Mixer-Blade Clearance in	Time	
1 Ala.	Twin shaft	1000	-	-	No	-
2 Ariz.	ditto	N.S. 1/	-	N.S.	No	-
3 Ark.	"	N.S.	-	3/4	No	-
4 Calif.	"	N.S.	70-90	N.S.	Yes	2
5 Colo.	"	N.S.	N.S.	N.S.	N.S.	N.S.
6 Conn.	"	750	-	1	No	-
7 Del.	"	N.S.	N.S.	2	Yes	-
8 D.of C.	"	1500	40	2	No	-
9 Fla.	"	N.S.	-	N.S.	No	-
10 Ga.	"	1000	-	3/4	No	-
11 Idaho	"	N.S.	N.S.	N.S.	No	-
12 Ill.	"	1000	55-75	3/4	Yes	5
13 Ind.	Batch	2000	-	3/4	Yes	-
14 Iowa	Twin shaft	-	-	3/4	Yes	5
15 Kans.	ditto	2000	N.S.	3/4	Yes	5
16 Ky.	"	2000	N.S.	2	Yes	5
17 La.	"	N.S.	56	N.S.	Yes	N.S.
18 Me.	"	1/2 rated capacity	As rated by manufacturer	-	Yes	-
19 Md.	"	1500	-	2	No	-
20 Mass.	"	52 cubic ft	-	2	No	-
21 Mich.	"	2000	60+	1	Yes	-
22 Minn.	"	N.S.	-	3/4	No	-
23 Miss.	Rotary drum or twin shaft	N.S.	N.S.	N.S.	Yes	-
24 Mo.	Twin shaft	2000	N.S.	3/4 (1-in.agg.)	Yes	N.S.
25 Mont.	ditto	Rated capacity	Produce uniform mix	3/4	Yes	-
26 Nebr.	"	N.S.	N.S.	N.S.	Yes	5
27 Nev.	"	N.S.	-	-	No	-
28 N.H.	"	2000	-	-	No	-
29 N.J.	"	1000	-	-	No	-
30 N.M.	"	-	As rated by manufacturer	1/2	Yes	10
31 N.Y.	"	2000	N.S.	3/4	Yes	5
32 N.C.	"	2000	N.S.	3/4	Yes	5
33 N.D.	Rotary drum or twin shaft	2000	N.S.	3/4 (1 1/2-in.agg.)	N.S.	-
34 Ohio	Twin shaft	2000	-	-	Yes	5
35 Okla.	ditto	1500	-	3/4 (1 1/2-in.agg.)	Yes	5
36 Oreg.	"	Depends on job tonnage	70-90	N.S.	No	-
37 Pa.	"	N.S.	Most effective speed	3/4	Yes	-
38 R.I.	"	Rated capacity	58-60	2	No	-
39 S.C.	"	-	-	2	No	-
40 S.Dak.	"	2000	60	2	No	-
41 Tenn.	"	2000	-	3/4	Yes	5-
42 Tex.	"	1500	N.S.	N.S.	Yes	N.S.
43 Utah	"	2000	N.S.	N.S.	Yes	-
44 Vt.	"	-	N.S.	N.S.	No	-
45 Va.	"	2000	40-60 rpm	1-1 1/2	No	-
46 Wash.	"	300 ton 18-hr. day	As rated by manufacturer	N.S.	No	-
47 W.Va.	"	2000	N.S.	N.S.	Yes	15
48 Wisc.	"	N.S.	N.S.	3/4	Yes	N.S.
49 Wyo.	"	N.S.	N.S.	3/4	Yes	-
50 Ontario	"	2000	-	3/4	N.S.	N.S.

1/ Not specified in specifications.

TABLE 11, PART III (continued)

Mixing Plant						
Type of Mixer Normally Used	Mixer (Continuous Plant)				Transport	
	Paddle Requirements				Truck Insulation	
	Usual Maximum Rate of Production tons per hour	Angular Adjustment	Capable of Reverse Motion	Minimum Allowable Capacity of Discharge Hopper lbs.	Cover Requirement	Type Specified
Twin pug	120	Yes	Yes	N.S.	Yes	-
ditto	125	Yes	No	N.S.	No	-
"	For satisfactory mix	Yes	No	N.S.	When req. by Engineer	-
"	For satisfactory mix	Yes	No	N.S.	Yes	Tarpaulins
"	N.S.	Yes	No	N.S.	Yes	Canvas
"	For satisfactory mix	Yes	Yes	N.S.	Yes	Waterproof canvas
"	50	-	Yes	N.S.	Yes - below 50°F	Canvas
"	120	Yes	Yes	-	Yes	-
"	N.S.	Yes	Yes	N.S.	Yes	Waterproof canvas
"	Screen capacity controls	Yes	Yes	-	Yes	Tarpaulins
"	50	Yes	-	One batch	No	-
"	40-120	Yes	Yes	2000	Yes	Canvas
"	-	Yes	Yes	-	Yes	Canvas
"	Mfr's. rated capacity	Yes	Yes	2000	Yes	-
"	Mfr's. rated capacity	Yes	Yes	2000	When req. by Engineer	-
"	Mfr's. rated capacity	Yes	Yes	N.S.	Yes	-
"	Type not used	-	-	-	Yes	-
"	-	-	-	-	Yes	Canvas
Twin pug	120	Yes	Yes	N.S.	Yes	-
ditto	N.S.	Yes	Yes	N.S.	Yes	-
"	Type not used	-	-	-	Yes	-
"	N.S.	No	No	N.S.	Yes	Waterproof canvas
"	80-100	Yes	Yes	N.S.	Yes	Canvas
"	N.S.	Yes	Yes	N.S.	Yes	Canvas
"	Mfr's. rated capacity	Yes	Yes	N.S.	Yes	As by Engineer
"	N.S.	Yes	No	200	Yes	-
"	-	-	-	-	Yes	-
Twin pug	Mfr's. rated capacity; min. of 80 tons per hr. Type not used	Yes	Yes	-	Yes	-
"	-	-	-	-	Yes	Canvas
Twin pug	Screen capacity controls	Yes	No	N.S.	No	-
"	-	-	-	-	Yes	Canvas
Twin pug	Mfr's. rated capacity	Yes	Yes	N.S.	Yes	Canvas
ditto	Mfr's. rated capacity	Yes	Yes	N.S.	Yes	-
"	-	Yes	No	-	Yes	-
"	N.S.	Yes	Yes	N.S.	Yes	-
"	N.S.	Yes	Yes	N.S.	As needed	-
"	For satisfactory mix	Yes	Yes	-	Yes	Canvas or heavy paper
"	Type not used	-	-	-	Yes	Canvas
"	For satisfactory mix	Yes	No	-	Yes	-
"	160	Yes	Yes	1000	In cool weather	-
"	-	Yes	Yes	-	Yes	Tarpaulin
"	N.S.	Yes	No	N.S.	In cool weather	Canvas
"	-	Yes	No	N.S.	Yes	Canvas
"	Plant size controls	Yes	No	N.S.	Yes	Canvas
"	Mfr's. rated capacity	Yes	No	N.S.	Yes	Tarpaulin
Twin, single	N.S.	No	No	N.S.	Yes	Tarpaulin
Twin pug	40	Yes	No	-	Yes	Waterproof canvas
ditto	120	Yes	Yes	N.S.	Yes	-
"	N.S.	Yes	Yes	N.S.	Yes	Canvas
Twin, single	N.S.	Yes	Yes	2000	Yes	-

TABLE 11, PART III (continued)

Station		Spreading and Finishing Machine						Placing	
Requirements		Device to Compensate for Irregularities						Use Screed Heater	
Insulation Required	Type Specified	Side Forms With	Side Forms Without	Leveling Used	Device to Compensate for Irregularities Not Used	Description	Yes	No	
No	-		x	-	-	-	x		
No	-		x		x	-		x	
No	-		x		x	-	x		
No	-		x	x		Adjustable screed	x		
-	-		x	x		Barber Greene - Adnum	x		
No	-		x		x	-	x		
Yes	-		x	x		Barber Greene	x		
Yes	-		x		x	-	x		
No	-		x		x	-	x		
No	-		x	x		Screed riding on compacted surface	x		
No	-	x		x		-	N S.		
Yes	3/4-in.		x	x		Barber Greene	x		
-	-		x	x		-	-	-	
No	-		x	x		Controlled by tracks on runners	x		
-	-		x	x		Self-leveling screed	x		
No	-		x		x	-	x		
No	-		x		x	-	x		
No	-		x	x	x	-	x		
No	-		x	x		-	-	-	
Below 50 F. or long haul	3/4-in.		x	-	-	Barber Greene - Adnum	Bar.Gr	x Adnum	
Yes - after Sept. 15th	1/2-in.		x	x		Equalizing runners, straight-edge runners, evener arms	x		
-	-		x	-	-	Barber Greene - Adnum	x		
No	-	x	x		x	-	x		
No	-		x	x		Barber Greene	x		
No	-		x		x	Barber Greene	x		
Yes	-		x	x		Screeds	x		
No	-		x		x	-	x		
Yes	-		x	x		Equalizing runners straight-edge runners, evener arms	-	-	
No	-	x	x		x	Activated strike-off	x		
-	-		x	x		Adjustable strike-off	x		
No	-		x	x		Equalizing runners, straight-edge runners, or evener arms	x		
No	-		x	x		Mechanical straight-edge runners, evener arms	x		
Yes	-		x	x		Leveling arms	x		
-	-		x	x		Delayed screed reaction	x		
No	-		x	x		Adjustable activated screed	x		
In cool weather When req by Engineer	Wood		x	x		10-ft runner	x		
-	-		x		x	Hand-screw mechanism	x		
No	-		x		x	-	x		
No	-		x	x		Barber Greene with crawler treads	x		
In cool weather When req by Engineer	-		x		x	Screed	x		
-	-		x		x	-	x		
No	-	x	x	x		Barber Greene	x		
-	-		x	x		Barber Greene	x		
No	-		x	x		Equalizing runners, straight-edge runners, evener arms	x		
-	-		x	x		Adjustable screed	x		
Yes	Celotex		x	x		Evener arms	x		
When req. by Engineer	-		x		x	-	x		
No	-		x		x	-	x		
No	-		x	x		Hinged floating screed	x		

TABLE 11, PART III (continued)

Compacting Rollers			1954 Practice
Types Required or Permitted: T-Tandem W=3 Wheel, P=Pneumatic	Specified Total Weight Limit	Specified Compression Weight	Agency
	tons	lbs./in. roller width	
T or W	5-10	330	1 Ala.
T or P	10-14	N.S.	2 Ariz.
T or W	7-10	200	3 Ark.
T, W or P	T 8, W 10	325	4 Calif.
T and W	T 5-8; W 10	N.S.	5 Colo.
T and W	10	N.S.	6 Conn.
T and W	T 8-10; W 10-12	250	7 Del.
T	8-12	200	8 D.of C.
T	8-10	200+	9 Fla.
T or W	T 7-10; W 10	200	10 Ga.
T	8+	N.S.	11 Idaho
T and W	8-12	250-400	12 Ill.
T and W	10+	300+	13 Ind.
T and W	8+	250+	14 Iowa
T or W	8-12	N.S.	15 Kans.
T or W	T 7; W 10	350 (W)	16 Ky.
T or W	N.S.	N.S.	17 La.
T	T 8-10	250	18 Me.
T	3-axle T 16-21		
N.S.	8+	200	19 Mi.
T	-	240-285	20 Mass.
	8+	-	21 Mich.
T and W	10+	250+	22 Minn.
T or W	T 7-10; W 10	200+	23 Miss.
T or W	8-12	200+	24 Mo.
T and W	10+	200+	25 Mont.
T and W	8-12	T 200; W 300	26 Nebr.
T	8-12	-	27 Nev.
T	8+	260+	28 N.H.
T and W	-	200	29 N.J.
T, W and P	8-10	325	30 N.M.
T or W	T 8-12; W 10-12	250	31 N.Y.
T	N.S.	250+	32 N.C.
T or W	5-10	200+	33 N.D.
T and W	T 8-12; W 10-12	-	34 Ohio
T, W, and P	N.S.	N.S.	35 Okla.
T or W	T 6; W 10	200	36 Oreg.
T and W	8-10	T 250; W 330	37 Pa.
T and W	10-12	N.S.	38 R.I.
T	8-10	250+	39 S.C.
T or W	10+	250+	40 S.Dak.
T and W	T 6-10; W 10	N.S.	41 Tenn.
T and W	T 8; W 10	N.S.	42 Tex.
T, W and P	10-14	N.S.	43 Utah
T	8+	-	44 Vt.
T and W	T 7-10; W 10-12	250	45 Va.
T or P	10	N.S.	46 Wash.
T or W	T 8-10; W 10	-	47 W. Va.
T or W	8-12	250	48 Wisc.
T, W or P	3-axle T 12-19	250 (P)	49 Wyo.
T or W	8+	T 200-250 W 310-350	50 Ontario



TABLE 12

## TESTS PERFORMED ON SAMPLES OF PLANT-PREPARED BITUMINOUS-CONCRETE MIXTURES

Agency	Tests Performed in Field Laboratory					Tests Per			
	Gradation	Extraction	1/ Density	Marshall	Others	Gradation	Extraction	1/ Density	Marshall
1 Ala.	L 2/	L, C 2/	C			L	L, C	C	
2 Ariz.	L					L	L		
3 Ark.	L	L				L	L	C	
4 Calif.	N 2/	N	C			L, C	L, C	L, C	
5 Colo.	L	L	C	N		L	L	C	
6 Conn.	L, C	L, C		L		L, C	L, C		L
7 Del.	L	L		C		L	L	C	
8 D. of C.	L					L	L	C	
9 Fla.	L	L	C		Compaction (L)		L	C	
10 Ga.	L	L	C		Hubbard-Field (L)	L	L	C	
11 Idaho	L	L			Moisture content (L)	L	L		
12 Ill.			C			L	L	C	L
13 Ind.		N	C			C	C		
14 Iowa	C		C			L, C	L, C	C	
15 Kans.	L, C	L, C	C			L			
16 Ky.	L	L	C				L		
17 La.	L, C	L	L, C	L		L, C	L	L, C	L
18 Me.	C	C	C			C	C	C	C
19 Md.	L					L	L	C	
20 Mass.	L					C	C	C	
21 Mich.	L	L				L	L		
22 Minn.	L, C					L, C	L, C	C	
23 Miss.	L, C	L, C	L, C	L				L, C	L
24 Mo.	L		C			L, C	L, C	C	
25 Mont.	L, C		C			L, C	C	L, C	
26 Nebr.		C	C			L	L	L	
27 Nev.							L, C		
28 N.H.	L	L				L	L	C	
29 N.J.	L, C	L, C	L, C			L, C	L, C	L, C	
30 N.M.	C	C	C	L		C	C	C	L
31 N.Y.	L	L				L	L		
32 N.C.	C	C	C			L	L	C	
33 N.Dak.	L		C		Thickness (C)		L	C	L
34 Ohio	L	L	C				L		
35 Okla.	L	L	L, C						
36 Oreg.	C	C					L, C	C	
37 Pa.	L	L					L		
38 R.I.	L					L	L	C	
39 S.C.	L, C	L, C				L, C	L, C	L, C	L
40 S.Dak.	L			L		L	L		L
41 Tenn.	L	L	C			L	L		
42 Tex.	L	L	L						
43 Utah	L	L	C			L	L		C
44 Vt.	L, C	L, C		C		L, C	L, C		L, C
45 Va.	L	L	C			L	L		C
46 Wash.	L					L	L	C	
47 W. Va.	C	C				C	C	C	
48 Wisc.	L		C			C	C		
49 Wyo.	L	L	C		Thickness (C)				
50 Ontario	C	C				C	C		

1/ Many agencies calculate the theoretical void content following the determination of density of sample.

2/ L - Sample of loose mixture.

C - Sample of compacted pavement.

N - Not known whether sample is of loose mixture or of compacted pavement.

TABLE 12 (continued)

1954 Practice

Formed in Central Laboratory					Minimum Frequency of Sampling Compacted Pavement for Density Test	Method of Removal of Density-Test Specimens From Pavement	Agency
Hveem Abilometer	Hubbard- Field	Abson Recovery	Thickness	Others			
				Hveem (L) cohesiometer	One per day Rarely One per 2000 tons One per mile  One each 4 hours One per day	Hand tools Not reported Hand tools Hand tools  Core Air hammer	1 Ala. 2 Ariz. 3 Ark. 4 Calif.  5 Colo. 6 Conn.
	L	L, C	C	Compaction (L) Moisture content (L)	Occasionally One per day One per day Seldom  One per day	Core Asphalt cutters Core Core -  Hand tools	7 Del. 8 D. of C. 9 Fla. 10 Ga. 11 Idaho  12 Ill. 13 Ind.
	C	C	C	Triaxial (L) compression	One or two per day One per day  One per day One per day One per 100 tons Each contract One per 1000 tons	Saw Hand tools  Hand tools Hand tools Core Saw Air hammer	14 Iowa 15 Kans.  16 Ky. 17 La. 18 Me. 19 Mi. 20 Mass.
	L L	C			None - Engr's discretion One per day One per day One per 200 tons One per day	- Air hammer Hand tools Saw Hand tools Hand tools Varied	21 Mich. 22 Minn. 23 Miss. 24 Mo. 25 Mont. 26 Nebr. 27 Nev.
			C	Unconfined (N) compression  Unconfined (N) compression	one per day  One per 15,000 s.y. or less laid each day Four per day None One per day	Saw, hand tools  Air hammer  Split ring - Cutting tool	28 N.H.  29 N.J. 30 N.M. 31 N.Y. 32 N.C.
			C		- Engr's discretion One per day Start of job - occa- sional check - - One per day	Hand tools Core Saw Core, hand tools  Core, saw Core Saw, hand tools	33 N.Dak. 34 Ohio 35 Okla. 36 Oreg.  37 Pa. 38 R.I. 39 S. C.
C	C	C		Swell (C) Hveem cohesiometer (L, C)	None Two per day None One per 5000 s.y. <sup>±</sup> - One per day -	- Cutting tool - Rings Core Core Core, hand tools	40 S.Dak. 41 Tenn. 42 Tex. 43 Utah 44 Vt. 45 Va. 46 Wash.
				Triaxial compression (C)	- Average one every other day Each shift -	Not reported Not reported  Hand tools Saw	47 W. Va. 48 Wisc.  49 Wyo. 50 Ontario

from the compacted pavement.

TABLE 13

## BASE PRIMING IN CONNECTION WITH BITUMINOUS CONCRETE CONSTRUCTION

Agency	Bituminous Grades Used for Prime Coat		Bituminous Grades Normally Used for Prime Coat		
	Asphalt	Tar	On Flexible Base	On Rigid Base	Grade Reported
1 Ala.	RC-1,2, MC-1,2	RT-1,2	RC-1,2; MC-1,2	RC-0,1, MC-0,1	--
2 Ariz.	MC-2	Not permitted	MC-2	No rigid base	MC-2
3 Ark.	RC-1; MC-0,1, Emulsion	Not permitted	MC-0,1	RC-1, Emulsion	MC-1
4 Calif.	SC-2, Pen. Emulsion	Not permitted	SC-2	Pen. Emulsion	SC-2
5 Colo.	MC-0	Not reported	Not reported	Not reported	MC-0
6 Conn.	No prime coat required				
7 Del.	RC-1, 3	Not permitted	RC-1	RC-3	
8 D. of C.	RC-2	Not reported	Not reported	RC-2	RC-2
9 Fla.	RC-1	RT-3, 4	RT-3, 4, RC-1	None	RC-1
10 Ga.	MC-1	Tar	Tar	Tar	MC-1
11 Idaho	RC-0,1, MC-0,1	Not permitted	Not reported	Not reported	RC-0, 1
12 Ill.	RC-0	RT-6	Not reported	RC-0	RC-0
13 Ind.	RC-1,2,3,4, Emulsion	Not permitted	RC-1,2,3,4 Emulsion	RC-3,4 Emulsion	
14 Iowa	RC-0	Not reported	Not reported	RC-0	RC-0
15 Kans.	RC-1; MC-2	Not permitted	MC-2	RC-1	MC-2
16 Ky.	RC-2, Emulsion	Tar	Tar	Emulsion	RC-2
17 La.	RC-1	Not permitted	RC-1	RC-1	RC-1
18 Me.	MC-0	Not reported	Not reported	Not reported	MC-0
19 Mi.	MC-1	Tar	Asphalt	Asphalt	MC-1
20 Mass.	RS-1	Not reported	Not reported	RS-1	RS-1
21 Mich.	MC-0, AE-2	T-3,4	MC-0	AE-2	MC-0
22 Minn.	RS, RC, MC-0,1,2	RT-1,2,3,4	Med. Curing Cut-Back	Emulsion Rapid Curing Cut-Back	MC-0,1,2
23 Miss.	MC-1	RT-2,3,4	MC-1	Not reported	MC-1
24 Mo.	MC-0 RC-0	Not permitted	MC-0	RC-0	RC-0
25 Mont.	MC-0,1	Not permitted	MC-1	MC-0	MC-1
26 Nebr.	RC-1, MC-1	Not permitted	MC-1	RC-1	MC-1
27 Nev.	MC-1	Not permitted	Not reported	Not reported	MC-1
28 N.H.	RS-1 MC-2	RT-3,4,5	Asphalt	RS-1	MC-2
29 N.J.	MC-0,1 RC-0 RS-1	RT-1,2	MC-0,1, RT-1,2	RC-0, RS-1	All
30 N.M.	MC-1	Not permitted	MC-1	None	MC-1
31 N.Y.	No prime coat required				
32 N.C.	MC-0 AE-7 RC-0	Not permitted	MC-0, RC-0, AE-7	MC-0, RC-0, AE-7	RC-0
33 N.Dak.	MC-0,1,2	Not permitted	MC-1	No rigid base	MC-0
34 Ohio	RC-1,2, MS-2	RT-1,2	RT-1,2	MS-2, RC-1,2	MC-1
35 Okla.	RC-1,2, MC-1, AE-5	Not permitted	MC-1	RC-1,2, AE-5	RC-1
36 Oreg.	RC-3; MC-2; RS-1	Not reported	MC-2, RC-3	RS-1	MC-1
					RS-1
					RC-3
					MC-2
37 Pa.	Asphalt, Emulsion	Tar	Tar	Asphalt	
38 R.I.	MC-2	T-2,3	RT-2,3	None	MC-2
39 S.C.	Asphalt	Tar	MC-0	Emulsion	
40 S.Dak.	RC-1, MC-1	Tar	MC-1	RC-1	MC-1
41 Tenn.	MC-1,2	Tar	Tar	MC-1,2	MC-1,2
42 Tex.	Emulsion RC-2, MC-2	Not permitted	MC-2	RC-2	MC-2
43 Utah	RC-1,2; MC-1,2	Not permitted	MC-1	RC-2	RC-1,2
44 Vt.	MC-2, RS-1	RT-5	Not reported	Not reported	MC-1,2
					RT-5
					MC-2
					RS-1
45 Va.	RC-2	Not reported	Cut-back	Cut-back	RC-2
46 Wash.	MC-3, Emulsion	Not reported	Not reported	Not reported	MC-3
47 W. Va.	AE M-1	RT-3,203	RT-3	AE M-1	
48 Wisc.	RS-1, RC-0,1, MC-0,1	Tar	MC-0, 1	RC-0,1, RS-1	MC-0
49 Wyo.	MC-0	Not reported	MC-0	Not reported	MC-0
50 Ontario	DHO Primer	Not permitted	DHO Primer	DHO Primer	DHO Primer

TABLE 13 (continued)

Reported Specifications for Prime-Coat Materials	
Required Physical Characteristics of Bituminous Material	
--	
AASHO M82-42 AASHO M82-42 AASHO M141-49	
AASHO M82-42	No prime coat required
	Not reported
AASHO M81-42 AASHO M81-42 except viscosity at 122°F. is 75-150 sec, and penetration at 77°F., 100 g., 5 sec. is 80-120. AASHO M82-42 AASHO M81-42 AASHO M82-42 AASHO M81-42 except flash point is 80°F.+	
	Not reported
AASHO M81-42 AASHO M82-42 except distillation test to 500°F. is 25 to 55, residue from dist. to 680°F. is 70+, and penetration @ 77°F., 100 g., 5 sec. is 150 to 225. AASHO M81-42	
AASHO M81-42 AASHO M82-42 except penetration at 77°F. 100 g., 5 sec. is 80 to 120. AASHO M82-42	
AASHO M140-49 AASHO M82-42	
AASHO M82-42	
AASHO M82-42 AASHO M81-42 AASHO M82-42	
AASHO M82-42 except no requirements are specified for the flash point.	Not reported
AASHO M82-42 AASHO Specifications AASHO M82-42 except residue from dist. to 680°F. is 63 to 73; & penetration @ 77°F., 100 g., 5 sec. is 120 to 220.	
	No prime coat required
AASHO M81-42 AASHO M82-42 AASHO M82-42 except viscosity @ 122°F is 75 to 100 AASHO M81-42 except flash point is 80+ AASHO M82-42 AASHO M140-49 AASHO M81-42 AASHO M82-42	
	Not reported
AASHO M82-42	Not reported
AASHO M82-42 AASHO M82-42 Flash point 150°F. +, viscosity @ 140°F. 100 to 200; distillation test 437°F. 0 to 2, 600°F. 10 to 20; residue from dist. to 680°F. 63+, penetration @ 77°F., 100 g. 5 sec. 100 to 200, ductility @ 77°F. 100+.	
AASHO M81-42 AASHO M82-42 AASHO M82-42 AASHO M82-42 AASHO M140-49 AASHO M81-42 except distillation test to 374°F. is 35+, to 437°F. is 65+, to 500°F. is 75+, & residue from dist. to 680°F. is 70+.	
AASHO M81-42 except the penetration @ 77°F., 100 g., 5 sec. is 120 to 220	Not reported
AASHO M82-42 except distillate to 600°F. is 75 to 93 AASHO M82-42	
Flash Point 80+, viscosity @ 122°F. 15 to 25, distillate to 374°F. 10+, 437°F. 16+, to 500°F. 20+, residue from dist. 680°F. 50+, penetration @ 77°F., 100 g., 5 sec., 100 to 200; ductility @ 77°F. 100, & bitumen soluble in C2S 99.5.	

TABLE 13 (continued)

Spot Test on Residue from Distillation			Application Rate (gallons)	
Standard Naphtha Solvent	Neg. with Naphtha Xylene Solvent (% Xylene)	Neg. with Heptane Xylene Solvent (% Xylene)	Flexible Base	Rigid Base
Yes	No	No	0.25-0.28	Not reported
--	--	35	0.5	No rigid base
Yes	--	--	0.3-0.4	0.03-0.10
--	--	35	0.15-0.25	Not a practice
	Not required		0.25 ±	0.10 approx.
	No prime coat required			
Neg.	Not required	--	0.2	0.1
	--	--	0.25-0.5	0.10
Neg.	Not required	--	0.2	0.06
--	--	35	0.15-0.50	0.15-0.50
Neg.	--	--	0.20-0.50	Not reported
Neg.	--	--	Not reported	0.05-0.10
Neg. or positive	Not reported		0.2-0.3	0.05-0.10
	Pos. -60% if pos. with Std. test		Not specified	0.12-0.15
	Not reported		0.25	0.25
Neg.	--	--	0.25 -	0.15 -
	Not reported		Not reported	0.17
	Not required		0.33-0.50	0.07
Neg.	Not reported	--	Not reported	0.07
	--	--	0.25(T-3 or MC-0)	0.10-0.15
Not required	10-(MC-2)	Not required	0.1-0.3	(Emulsion) 0.03-0.10
Neg.	--	--	0.15-0.50	Not specified
Neg.	--	--	0.2 - 0.5	0.02-0.1
--	Not required	--	0.15-0.25	0.1 -
	10	--	0.25-0.30	0.04-0.10
	Not reported		0.375	Not reported
	Not reported		0.5	0.15 +
	Not required	--	0.1-0.25	0.10-(RC-0)
--	15	--	0.25-0.5	None
	No prime coat required			
	Not reported		0.3	0.06-0.12
Neg.	Not required	--	0.35	No rigid base
	Not reported		0.25-0.35	0.10 -
	--		0.25	0.1
	Not required		0.25-0.50	0.1-0.2
	Not reported		0.15-0.25	0.05-0.07
	Not required		0.33	None
--	Not required	--	0.1 approx	0.1 approx
Neg.	15	--	0.4	0.08
Yes	--	--	0.15-0.45	0.05-0.15
	--	--	0.25	0.03
--	--	35	0.25-0.50	0.08-0.15
	Not reported		0.3-0.4	0.1
Neg.	--	--	0.1	0.05
--	--	35	0.25	0.02-0.05
	Not reported	--	0.30-0.60	0.15-0.25
Neg.	--	--	0.1-0.35	0.03-0.1
--	15	--	0.4	Not reported
	Not required		0.17-0.25	Not specified

TABLE 13 (continued)

1954 Practice

Application of Prime Coat			Agency
per sq. yd.) Method of Control	Application Temperature (°F.)	Required Curing Period	
Tachometer	120-140	3 days	1 Ala.
Tachometer	150-200	Until penetrated or blotted	2 Ariz.
Tachometer	50 -125	Not specified	3 Ark.
Tachometer	150-225	Not specified	4 Calif.
Synchronizer			
Tachometer	120 -	24 hours	5 Colo.
No prime coat required			6 Conn.
Tachometer	Not specified	Several hours	7 Del.
Tachometer	125-175	Not reported	8 D. of C.
Tachometer	100-150	Not specified	9 Fla.
Tachometer	100-160	Not specified	10 Ga.
Tachometer	150	Not specified	11 Idaho
meter-vol.			
Tachometer	Not specified	Until no pick-up under traffic	12 Ill.
	Not reported		13 Ind.
Tachometer	80- 90	24 hours	14 Iowa
Tachometer	125-200	Not specified	15 Kans.
Visual inspection	Not reported	Not reported	16 Ky.
measure & calculate			
Tachometer	Not specified	Not specified	17 La.
Tachometer	Air temperature	1 hour +	18 Me.
Tachometer	120 -	24 hours +	19 Md.
Not reported	60 - 120	Not reported	20 Mass.
Tachometer	50-120 (MC-0)	48 hours (MC-0)	21 Mich.
	60-175 (Emulsion)	1000-1500 ft. ahead (Emulsion)	
Tachometer	80-125(MC-0) 60-125 RT-1,2)	Until no pick-up under traffic	22 Minn.
	100-175(MC-1) 80-150 RT-3,4)		
	150-200 (MC-2)		
Tachometer	175 -	Not specified	23 Miss.
Tachometer	80-120	Until properly cured	24 Mo.
Tachometer	100-175	24 hours +	25 Mont.
Tachometer	Not specified	Not specified	26 Nebr.
Tachometer	Not reported	Not reported	27 Nev.
Tachometer	Not specified	24 hours +	28 N. H.
Tachometer	50-120	Until properly cured	29 N. J.
Tachometer	125-200	24 hours	30 N. M.
No prime coat required			31 N. Y.
Tachometer	90-130	Until properly cured	32 N. C.
Tachometer	75-200	2 - 3 days	33 N. Dak.
Tachometer	Not reported	Not reported	34 Ohio
Tachometer	75-120	Until properly cured	35 Okla.
Tachometer, pressure	150-175	72 hours	36 Oreg.
& volume gage			
Tachometer	175 -	Until tacky	37 Pa.
Tachometer	120	Not reported	38 R. I.
Tachometer	Not specified	Until tacky	39 S. C.
Tachometer	150 -	24 hours	40 S. Dak.
Tachometer	100-150	Until properly cured	41 Tenn.
Tachometer	140	12 hours	42 Tex.
Tachometer	150-200	Not specified	43 Utah
Tachometer	140-150 (tar)	7 days except emulsion on conc.	44 Vt.
	150-160 (MC-2)		
Tachometer	140-160	Until tacky	45 Va.
Tachometer	50 +	Not specified	46 Wash.
Tachometer	80-150	Not reported	47 W. Va.
Tachometer	100-120	24-48 hours	48 Wisc.
Tachometer	100-200	24 hours	49 Wyo.
Synchronizer			
Tachometer	70-100	Not specified	50 Ontario

TABLE 14  
THICKNESS OF PAVEMENTS INVOLVING A BITUMINOUS CONCRETE SURFACE

Agency	Design Method Used to Determine Thickness of Flexible Pavements	Use of Subgrade Soil Characteristics to Determine Thickness of Flexible Pavement
1 Ala	Not reported	Not reported
2 Ariz	Consider PI and amount of minus No 200 sieve material in subgrade soil	Total thickness based on PI and amt of minus No 200 sieve material in subgrade soil. Some characteristics of subbase material determine subbase and base thickness
3 Ark	Consider HRB soil classification of subgrade soil	HRB soil classification of subgrade soil determines subbase thickness
4 Calif	California Method - consider stabilometer "Resistance Value" of base and volume and magnitude of traffic	Shearing resistance and expansive characteristics of soil evaluated
5 Colo	Colorado Method - consider soil CBR and moisture condition, traffic, and climate	Consider CBR
6 Conn	Past experience - consider soil type frost penetration, ground water, and traffic	Subgrade soil type considered in determining subbase thickness
7 Del	Consider CBR and frost penetration	Consider CBR of subgrade soil in determining subbase thickness
8 D of C	Past experience	Not reported
9 Fla	Past experience - consider traffic	Subgrade soil characteristics not considered
10 Ga	Not reported	Not reported
11 Idaho	Hveem Method	Hveem Method
12 Ill	Consider HRB soil classification, traffic, drainage, and frost penetration	Consider HRB soil classification
13 Ind	Not reported	Not reported
14 Iowa	Not reported	Not reported
15 Kans	Kansas Triaxial Method	Consider modulus of deformation from triaxial compression test
16 Ky	Consider CBR	Consider CBR
17 La	Not reported	Not reported
18 Ma	Consider volume and type of traffic	Subgrade soil characteristics not considered
19 Md	Consider HRB soil classification and CBR	Consider HRB soil classification and CBR in determining total thickness
20 Mass	Consider volume and type of traffic	Subgrade soil characteristics may influence choice of subbase thickness
21 Mich	Consider traffic in surfacing design. Consider soil profile classification and estimated stability in foundation design	Consider estimated spring CBR
22 Minn	Consider CBR (modified test), and rely on past experience	Thicknesses modified on basis of HRB soil classification
23 Miss.	Consider CBR (modified test), of pavements designed to carry wheel loads of over 9000 lbs	Consider CBR
24 Mo	Consider HRB soil classification and traffic volume	Consider HRB group index
25 Mont	Consider HRB soil classification	Consider HRB soil classification
26 Nebr	Consider traffic, rainfall, drainage and HRB group index of subgrade soil	Consider HRB group index
27 Nev	Consider HRB soil classification	Consider HRB soil classification
28 N H	Past experience	Subgrade soil type influences choice of subbase thickness
29 N J	Past experience	Thickness increased for A-6 to A-8 subgrades
30 N M	Consider traffic and rainfall, and gradation and Atterberg limits of base and subbase material	Consider soil type
31 N Y	Rational determination	Knowledge of previous behavior
32 N C	Consider traffic and bearing value of subgrade	Consider bearing value of subgrade in determining total thickness
33 N Dak	North Dakota Method - consider North Dakota cone test values and subgrade soil type	Subgrade soil type and North Dakota cone value of subgrade soil considered in determining subbase thickness
34 Ohio	Not reported	Not reported
35 Okla	Consider CBR	Consider CBR of subgrade soil in determining subbase thickness
36 Oreg	Triaxial - modified Hveem Method	Consider "R" value (from vertical and horizontal pressure ratio) and silt content
37 Pa	Not reported	Not reported
38 R I	Past experience	Non-drainable material usually removed
39 S C	Past experience	Not reported
40 S Dak	Past experience	Evaluate bearing ability
41 Tenn	Past experience	Evaluate bearing ability
42 Texas	Triaxial tests of pavement and subgrade material	Consider shear strength as determined by triaxial method
43 Utah	Experience and "R" value from Hveem stability test	Consider subgrade characteristics in determining base and subbase thickness
44 Vt	Bituminous concrete used mostly to resurface existing RCC pavements	Not reported
45 Va	Consider CBR (modified)	Total thickness related to strength of subgrade as indicated by modified CBR
46 Wash	Consider test values from Hveem Stabilometer and swell-pressure tests	Total thickness related to Hveem Stabilometer and swell-pressure test values
47 W Va	Ky design curves (CBR) and Ohio design curves (HRB class)	Total thickness determined from design curves
48 Wisc	Consider traffic volume and soil type	Consider load-carrying capacity as affected by drainability
49 Wyo	Consider CBR (modified) and test values from Hveem Stabilometer	Consider CBR (modified) and test values from Hveem Stabilometer - add extra cover on frost-reactive materials
50 Ontario	Past experience - consider results of mechanical analysis and plate-bearing tests	Consider results of mechanical analysis and plate-bearing tests

- 1/ The given conditions do not occur, or occur infrequently, in some areas of the country. However, some of the agencies in these areas have listed the thicknesses that their design methods would indicate to be satisfactory.
- 2/ Thickened edges

TABLE 14 (continued)

Average Thicknesses (in inches) Likely to be Used										
No Differentiation as to Traffic										
Rigid Base					Flexible Base					
Subbase	Base	Binder	Surface	Total	Subbase	Base	Binder	Surface	Total	Subbase
										10
										6½
										-
8+	8	1 1/8	1 1/8	18½+	12	8	1½	1	22½	
										6
										3
12	-	-	-	-	4-6 12	2-10 4½	2 1½	1½ 1½	- 19	
-	-	1½	1½	-	6	8	2½	1½	18	12 6
	7	-	3	10	11	2	1½	1½	16	
-	-	2	2	-	- 0-13	- 3	2 2	2 2	- 5-18	
										12
4	-	-	-	-	5 6	2 8	- -	2½ -	9½ -	
6-12	6-8	1½	1½	15-23	6-18 4-12 -	5-6 4-8 6	1½ 1-1½ 4	1½ 1½-2 1½	14-27 10½-23½ 11½	6
					8	6	2½	1½	18	12½



TABLE 14 (continued)

ed Under These Conditions: 1/ Subgrade Soil A-6, Average Annual Rainfall 32 Inches, Average Ann Heavy-Traffic Pavement									
Rigid Base				Flexible Base					
Base	Binder	Surface	Total	Subbase	Base	Binder	Surface	Total	Subbase
-	-	-	-	10 12-18	10 3	-	- 2½	- 17½-23½	6
				12	12	3	1½	28½	
8	1½	1½	17½	13	8	1½	1½	24	4
8	1½	1½	11	20	4	1½	1½	27	-
				20(cut) 12 (fill) 9	6 8	1½ 2	1½ 1½	28½(cut) 20½(fill) 20½	
				0-18 7	5-18 10	- 1½	3 1½	- 20	
6	1½	1½	15	8	6	1½	1½	17	0
7	1½	1½	13	-	12	1½	1½	15	
				24-36	6	1	1	32-38	
				-	4½	-	-	-	
8	1 7	1 3	23	24	10	1 7	1 3	37	12
-	1½	1½	-	15	9+	2	2	28	-
				-	8	1 3/4	1½	11	
				4	3	-	3	10	
				0-12	24	2	1	27-39	
				3-13	3	0	2	8-18	
3-9	1½	1	22½	12	7	1½	1	21½	
				0-6	5-14	1½	1½	17	4
				5+	2	-	2½	9½+	
					12-21	2	1½	15½-24½	
10	0	1	17	9 8-12	8 3-6	0 2	1 1	18 14-21	6
				6-10	6-10	1½	1-1½	14½-23	
4	2	1	19½	17	4	2	1	24	10
				6-9 10½	7-14 2/6½-5-6½	1½ 1½	1½ 1½	19-26 2/19½-18-19½	
				18-20	4	3½	1½	29	

TABLE 14 (continued)

1954 Practice									Agency
Medium-Traffic Pavement									
Rigid Base				Flexible Base					
Base	Binder	Surface	Total	Subbase	Base	Binder	Surface	Total	
-	-	-	-	6 6-15	8 3	-	- 2½	- 11½-20½	1 Ala 2 Ariz
				8-12	8-10	2	1½	19½-25½	3 Ark
6	1½	1½	13	10	6	1½	1½	19	4 Calif
6	1½	1½	9	15	4	1½	1½	22	5 Colo
				15(cut) 12(fill) 7	6 6	1½ 2	1½ 1½	23½(cut) 18½(fill) 16½	6 Conn 7 Del
				0-18 7	5-18 9	- 1½	2½ 1½	7½-38½ 19	8 D of C 9 Fla 10 Ga
6	1½	1½	8½	0	7	1½	1½	9½	11 Idaho 12 Ill 13 Ind 14 Iowa 15 Kans
				- 18-24	8 -	1½ 2	1½ 1	11 21-27	16 Ky 17 La 18 Me 19 Md
				12	3	1½	1½	-	20 Mass
8	-	2	22	18	8	-	2	28	21 Mich
-	1½	1½	-	12	6+	1½	1½	21	22 Minn 23 Miss
				-	6	1 3/4	1½	9	24 Mo 25 Mont 26 Nebr
				3	2	-	2	7	27 Nev 28 N H 29 N J 30 N M
				0-12	18	2	1	21-33	31 N Y 32 N C
				0-13	3	0	2	5-18	
-	-	-	12	12 0-10	4 7-10	1½ 0-2	1 1	18½ 11	
				5	2	-	2½	9½	33 N Dak 34 Ohio 35 Okla
				-	7-12	2	1½	10½-15½	36 Oreg
6-8	1½	1½	9-11	6-12	5½-8	1½	1½	8½-9	37 Pa 38 R I 39 S C 40 S Dak
9	0	1	16	8	7	0	1	16	41 Tenn 42 Texas 43 Utah
				4-6	4-6	1	1	10-14	44 Vt
4	1½	1	16½	14½	4	1½	1	21	45 Va 46 Wash
				6-9 9	6-10 4-5½	1½ 1	1 1	14½-21½ 15-16½	47 W Va 48 Wisc 49 Wyo
				12-14	4-6	2-4	1½	19½-25½	50 Ontario